

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090822\
 Data File : VV027791.D
 Acq On : 08 Sep 2022 15:57
 Operator : SY/MD
 Sample : VV0908WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Quant Time: Sep 09 03:00:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 09 02:55:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	4454	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.848	117	4169	0.500	ug/L	-0.01
11) 1,4-Dichlorobenzene-d4	11.244	152	2923	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	1510	0.547	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	110.000%
4) 1,2-Dichloroethane-d4	5.042	65	1102	0.530	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
7) 1,2-Dichloropropane-d6	6.068	67	709	0.511	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.000%
8) Toluene-d8	7.317	98	4031	0.524	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
10) 1,1,2,2-Tetrachloroeth...	10.199	84	632	0.531	ug/L	-0.02
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.324	75	7	0.036	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090822\
Data File : VV027791.D
Acq On : 08 Sep 2022 15:57
Operator : SY/MD
Sample : VV0908WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Time: Sep 09 03:00:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM090822.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 09 02:55:15 2022
Response via : Initial Calibration

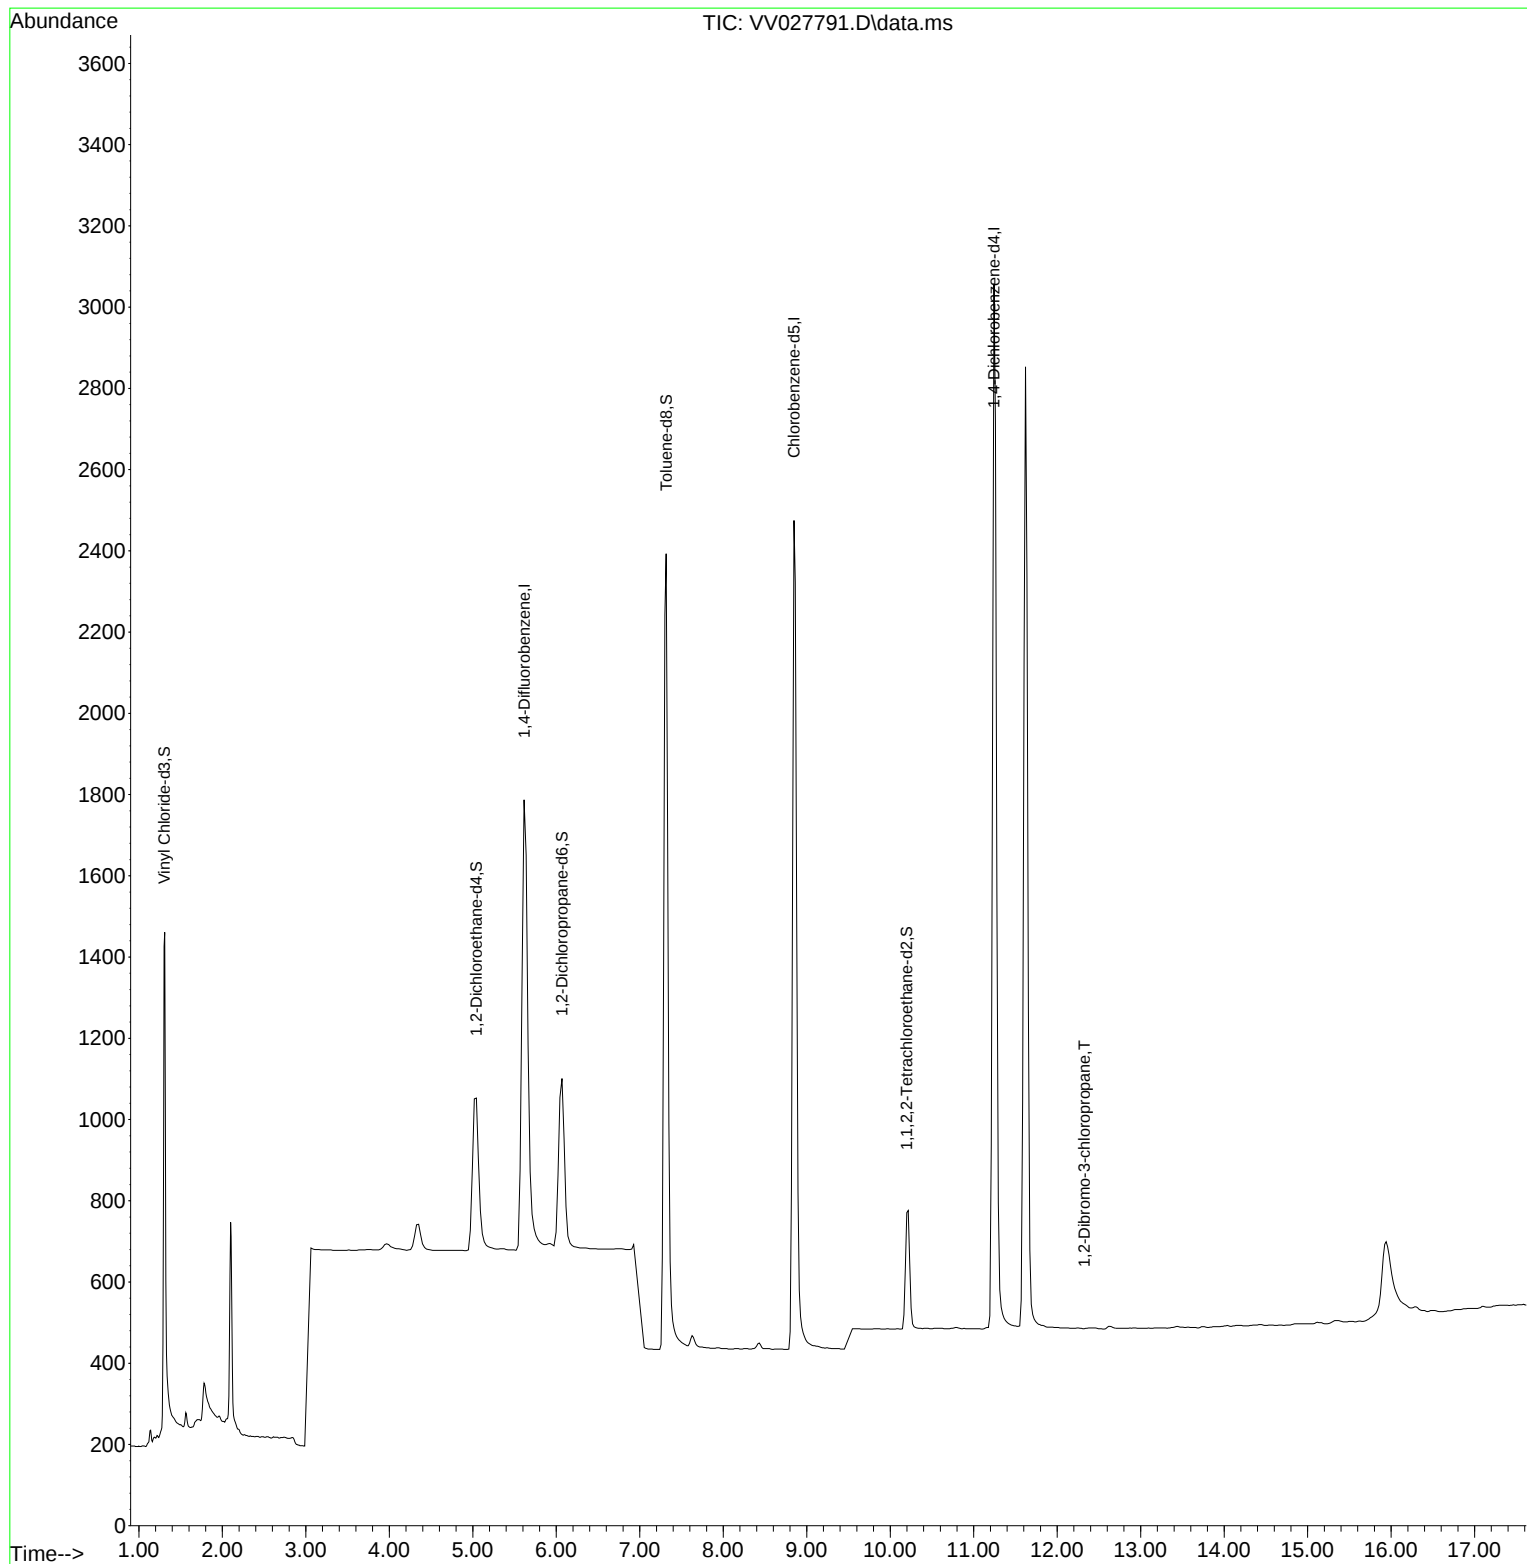

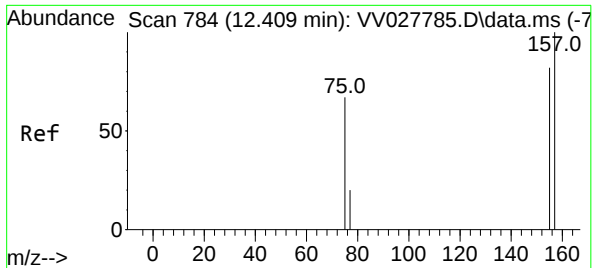

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.036 ug/L
 RT: 12.324 min Scan# 71
 Delta R.T. -0.086 min
 Lab File: VV027791.D
 Acq: 08 Sep 2022 15:57

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Tgt Ion: 75	Resp:	7
Ion	Ratio	Lower Upper
75	100	
157	98.0	94.2 141.2
155	98.0	86.1 129.1

