

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031976.D
 Acq On : 08 Sep 2023 11:24
 Operator : SY/MD
 Sample : VV0908WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 09 05:34:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 09 05:33:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	300131	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	288191	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	149421	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	98087	52.220	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	104.440%
7) Chloroethane-d5	1.529	69	78508	47.680	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.360%
11) 1,1-Dichloroethene-d2	2.056	65	42623	48.461	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.920%
21) 2-Butanone-d5	3.789	46	147245	99.672	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.670%
24) Chloroform-d	4.252	84	180416	43.945	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.880%
26) 1,2-Dichloroethane-d4	4.944	65	120914	44.379	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.760%
32) Benzene-d6	4.963	84	382914	48.693	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.380%
36) 1,2-Dichloropropane-d6	5.992	67	127605	50.414	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.820%
41) Toluene-d8	7.246	98	353033	48.722	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.440%
43) trans-1,3-Dichloroprop...	7.555	79	62882	47.932	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.860%
47) 2-Hexanone-d5	8.027	63	100350	129.353	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	129.350%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	158905	48.583	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.160%
66) 1,2-Dichlorobenzene-d4	11.564	152	130687	47.978	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.960%
Target Compounds						
39) cis-1,3-Dichloropropene	6.918	75	3632	0.952	ug/L	Qvalue # 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031976.D
Acq On : 08 Sep 2023 11:24
Operator : SY/MD
Sample : VV0908WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 09 05:34:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 09 05:33:49 2023
Response via : Initial Calibration

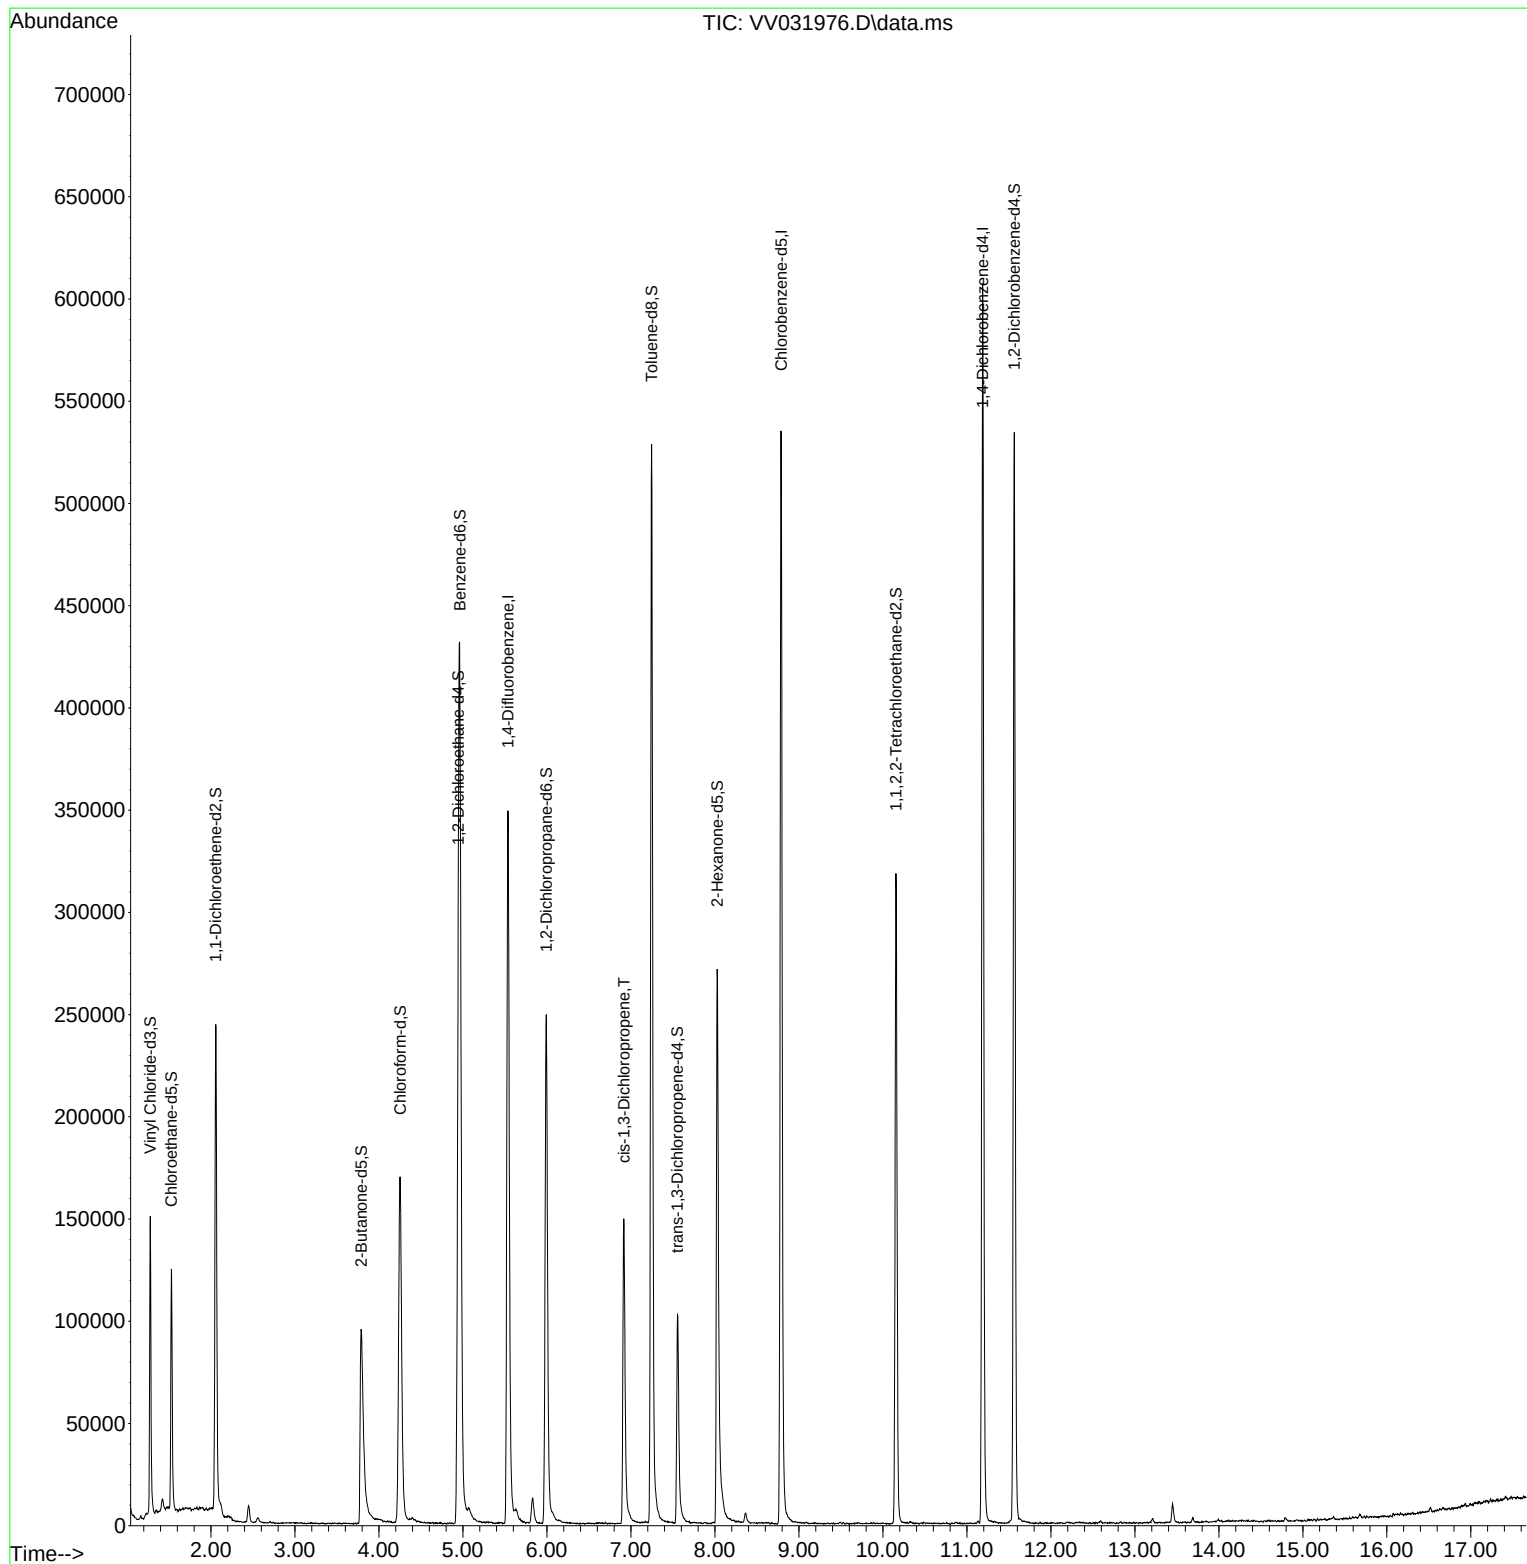

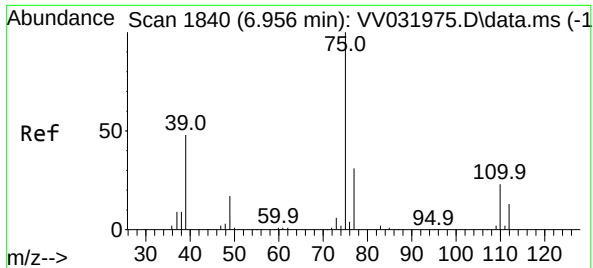

#39
 cis-1,3-Dichloropropene
 Concen: 0.952 ug/L
 RT: 6.918 min Scan# 11
 Delta R.T. -0.038 min
 Lab File: VV031976.D
 Acq: 08 Sep 2023 11:24

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3632
 Ion Ratio Lower Upper
 75 100
 77 55.2 21.4 39.8#

