

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031976.D
 Acq On : 08 Sep 2023 11:24
 Operator : SY/MD
 Sample : VV0908WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

Signal : TIC: VV031976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	145291	159066	14.00%	1.760%
2	1.529	145	152	168	rVB	118128	142607	12.55%	1.578%
3	2.056	307	316	349	rVB	241001	381260	33.56%	4.218%
4	2.449	430	438	450	rVB2	7960	13156	1.16%	0.146%
5	2.513	456	458	461	rBV4	373	284	0.03%	0.003%
6	2.558	465	472	480	rVV5	1851	3393	0.30%	0.038%
7	2.703	514	517	522	rVB4	727	716	0.06%	0.008%
8	2.741	527	529	536	rVB4	703	648	0.06%	0.007%
9	2.773	536	539	541	rBV3	453	350	0.03%	0.004%
10	3.089	635	637	642	rVB3	442	314	0.03%	0.003%
11	3.725	832	835	838	rVB3	635	360	0.03%	0.004%
12	3.748	838	842	844	rBV4	519	333	0.03%	0.004%
13	3.789	845	855	901	rBV2	95052	282516	24.87%	3.125%
14	4.252	981	999	1031	rBV	169064	435564	38.34%	4.818%
15	4.542	1086	1089	1094	rVB6	640	493	0.04%	0.005%
16	4.635	1115	1118	1121	rBV2	428	302	0.03%	0.003%
17	4.722	1142	1145	1148	rVV4	571	369	0.03%	0.004%
18	4.738	1148	1150	1156	rVB6	867	675	0.06%	0.007%
19	4.818	1172	1175	1178	rBV3	436	328	0.03%	0.004%
20	4.844	1178	1183	1187	rVV4	636	644	0.06%	0.007%
21	4.870	1187	1191	1196	rVB5	555	518	0.05%	0.006%
22	4.960	1201	1219	1245	rBV2	431061	1135924	100.00%	12.566%
23	5.252	1308	1310	1314	rVB3	685	454	0.04%	0.005%
24	5.278	1314	1318	1321	rBV4	709	602	0.05%	0.007%
25	5.397	1352	1355	1359	rVB4	531	446	0.04%	0.005%
26	5.487	1380	1383	1385	rBV3	418	279	0.02%	0.003%
27	5.535	1385	1398	1420	rBV	348570	722792	63.63%	7.996%
28	5.760	1466	1468	1477	rVB4	511	667	0.06%	0.007%
29	5.831	1477	1490	1506	rBV	12247	26630	2.34%	0.295%
30	5.992	1525	1540	1576	rBV	248983	529440	46.61%	5.857%
31	6.397	1663	1666	1668	rBV3	603	409	0.04%	0.005%
32	6.423	1668	1674	1676	rBV3	313	305	0.03%	0.003%
33	6.432	1676	1677	1681	rVB3	522	299	0.03%	0.003%
34	6.458	1681	1685	1688	rBV4	466	431	0.04%	0.005%
35	6.622	1733	1736	1741	rVV4	520	442	0.04%	0.005%
36	6.654	1743	1746	1752	rVB3	429	333	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031976.D
 Acq On : 08 Sep 2023 11:24
 Operator : SY/MD
 Sample : VV0908WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.699	1758	1760	1763	rVB2	707	328	0.03%	0.004%
38	6.915	1816	1827	1861	rBV	149135	288890	25.43%	3.196%
39	7.172	1905	1907	1910	rBV	618	343	0.03%	0.004%
40	7.246	1918	1930	1961	rBV	527315	945831	83.27%	10.463%
41	7.555	2016	2026	2051	rBV	101928	188898	16.63%	2.090%
42	7.735	2080	2082	2085	rBV5	422	283	0.02%	0.003%
43	7.876	2119	2126	2128	rBV5	589	693	0.06%	0.008%
44	7.937	2142	2145	2148	rBV4	328	318	0.03%	0.004%
45	7.979	2152	2158	2159	rBV4	599	560	0.05%	0.006%
46	8.027	2164	2173	2204	rBV	270970	516535	45.47%	5.714%
47	8.365	2269	2278	2290	rBV3	4483	7858	0.69%	0.087%
48	8.522	2322	2327	2330	rBV3	652	748	0.07%	0.008%
49	8.558	2335	2338	2342	rVB3	688	512	0.05%	0.006%
50	8.677	2371	2375	2379	rVV4	778	541	0.05%	0.006%
51	8.786	2396	2409	2429	rBV	534767	893968	78.70%	9.889%
52	9.079	2496	2500	2501	rBV3	459	312	0.03%	0.003%
53	9.191	2531	2535	2537	rBV3	645	456	0.04%	0.005%
54	9.342	2578	2582	2586	rVV3	422	378	0.03%	0.004%
55	9.384	2591	2595	2598	rBV4	347	350	0.03%	0.004%
56	9.410	2600	2603	2608	rVB2	564	409	0.04%	0.005%
57	9.529	2635	2640	2645	rVB4	721	761	0.07%	0.008%
58	9.612	2663	2666	2667	rBV2	415	289	0.03%	0.003%
59	9.866	2742	2745	2748	rVB2	550	338	0.03%	0.004%
60	9.886	2748	2751	2753	rBV2	582	420	0.04%	0.005%
61	9.924	2759	2763	2766	rBV	340	305	0.03%	0.003%
62	10.056	2800	2804	2806	rBV2	419	302	0.03%	0.003%
63	10.156	2821	2835	2858	rVV	317985	511823	45.06%	5.662%
64	10.288	2873	2876	2881	rVB3	543	301	0.03%	0.003%
65	10.320	2882	2886	2889	rBV4	696	588	0.05%	0.007%
66	10.368	2899	2901	2905	rVB2	478	283	0.02%	0.003%
67	10.391	2905	2908	2911	rBV3	508	294	0.03%	0.003%
68	10.484	2935	2937	2945	rVB5	716	830	0.07%	0.009%
69	10.603	2972	2974	2977	rBV3	490	357	0.03%	0.004%
70	10.760	3019	3023	3025	rBV3	620	363	0.03%	0.004%
71	10.815	3036	3040	3042	rBV3	648	447	0.04%	0.005%
72	10.863	3050	3055	3058	rBV4	758	803	0.07%	0.009%
73	10.969	3084	3088	3090	rBV2	500	350	0.03%	0.004%
74	11.127	3133	3137	3138	rBV3	1020	612	0.05%	0.007%
75	11.188	3145	3156	3181	rBV	606406	950036	83.64%	10.510%
76	11.564	3253	3273	3290	rBV	533288	846238	74.50%	9.361%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031976.D
 Acq On : 08 Sep 2023 11:24
 Operator : SY/MD
 Sample : VV0908WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.754	3330	3332	3338	rVB3	409	300	0.03%	0.003%
78	11.870	3364	3368	3369	rBV	721	552	0.05%	0.006%
79	11.937	3382	3389	3393	rBV4	666	979	0.09%	0.011%
80	12.194	3462	3469	3474	rVV5	685	1016	0.09%	0.011%
81	12.458	3547	3551	3553	rBV2	546	364	0.03%	0.004%
82	12.532	3572	3574	3577	rBV3	659	469	0.04%	0.005%
83	12.567	3581	3585	3587	rBV3	553	528	0.05%	0.006%
84	12.873	3678	3680	3687	rVV4	544	455	0.04%	0.005%
85	12.902	3687	3689	3695	rVV5	438	334	0.03%	0.004%
86	12.940	3700	3701	3706	rVB3	578	377	0.03%	0.004%
87	12.985	3711	3715	3718	rVB4	590	327	0.03%	0.004%
88	13.017	3723	3725	3733	rVB5	563	603	0.05%	0.007%
89	13.059	3735	3738	3747	rVB4	508	652	0.06%	0.007%
90	13.181	3770	3776	3778	rBV4	696	709	0.06%	0.008%
91	13.210	3778	3785	3794	rVB8	2312	3655	0.32%	0.040%
92	13.358	3829	3831	3834	rBV2	464	332	0.03%	0.004%
93	13.448	3851	3859	3870	rBV	9017	14206	1.25%	0.157%
94	13.541	3886	3888	3894	rVB4	539	454	0.04%	0.005%
95	13.570	3894	3897	3901	rBV4	693	644	0.06%	0.007%
96	13.625	3912	3914	3917	rBV4	487	381	0.03%	0.004%
97	13.693	3928	3935	3946	rVB6	2272	3491	0.31%	0.039%
98	13.738	3946	3949	3950	rBV2	467	298	0.03%	0.003%
99	14.352	4137	4140	4142	rVB3	723	363	0.03%	0.004%
100	14.535	4195	4197	4202	rBV3	679	789	0.07%	0.009%




Sum of corrected areas: 9039578

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031976.D
Acq On : 08 Sep 2023 11:24
Operator : SY/MD
Sample : VV0908WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

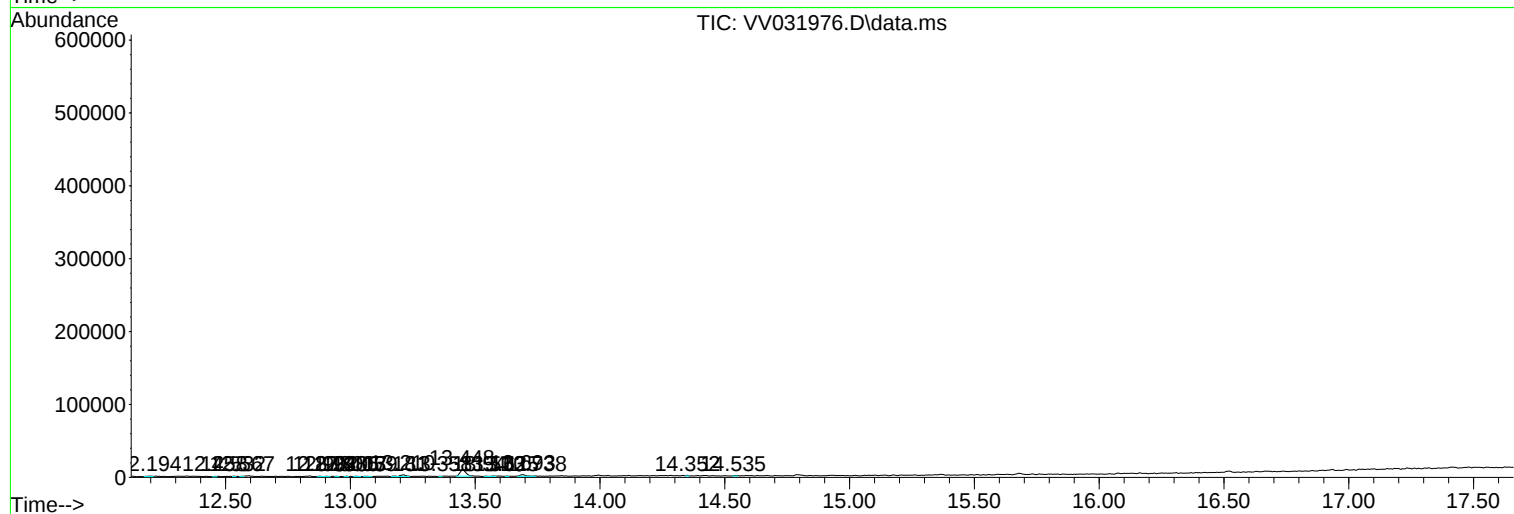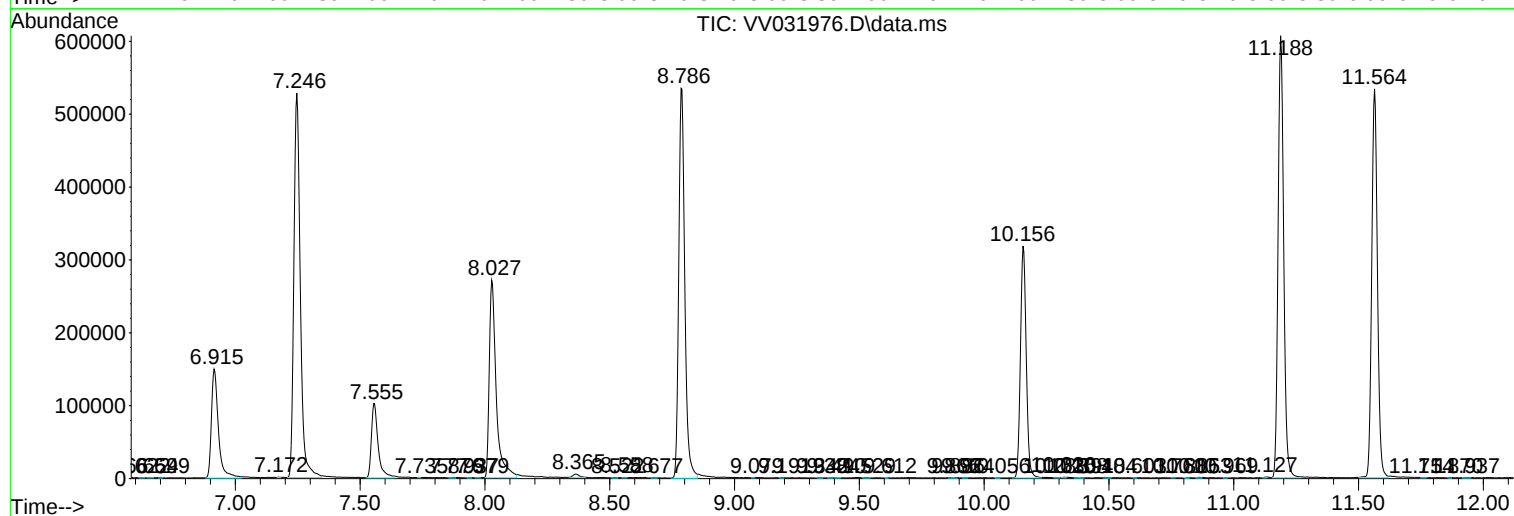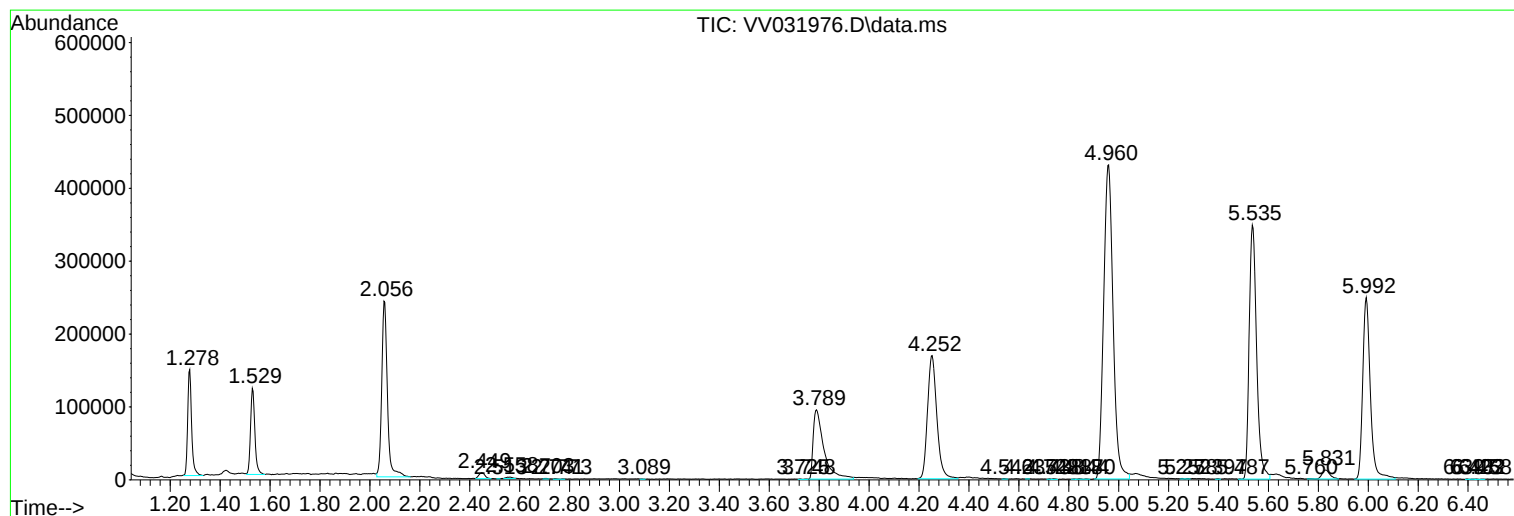

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031976.D
Acq On : 08 Sep 2023 11:24
Operator : SY/MD
Sample : VV0908WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031976.D
Acq On : 08 Sep 2023 11:24
Operator : SY/MD
Sample : VV0908WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------