

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031983.D
 Acq On : 08 Sep 2023 16:09
 Operator : SY/MD
 Sample : VIBLK229
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	100866	106537	11.43%	1.492%
2	1.529	146	152	173	rVB	89630	112719	12.09%	1.578%
3	2.060	309	317	333	rVB	161610	230910	24.77%	3.233%
4	2.449	432	438	454	rVB	8930	14799	1.59%	0.207%
5	3.150	655	656	662	rVB3	549	438	0.05%	0.006%
6	3.294	698	701	706	rVB4	778	440	0.05%	0.006%
7	3.372	722	725	727	rVB	349	182	0.02%	0.003%
8	3.391	727	731	733	rBV2	531	391	0.04%	0.005%
9	3.458	750	752	756	rVB	454	228	0.02%	0.003%
10	3.532	772	775	777	rBV	337	213	0.02%	0.003%
11	3.687	821	823	827	rVB3	449	314	0.03%	0.004%
12	3.716	827	832	834	rBV2	279	236	0.03%	0.003%
13	3.793	845	856	901	rBV2	96314	297655	31.93%	4.168%
14	4.256	984	1000	1025	rBV	136312	351558	37.72%	4.923%
15	4.719	1140	1144	1147	rVB3	560	426	0.05%	0.006%
16	4.857	1185	1187	1190	rBV3	332	223	0.02%	0.003%
17	4.960	1203	1219	1247	rBV2	352446	932071	100.00%	13.051%
18	5.204	1292	1295	1298	rBV5	637	491	0.05%	0.007%
19	5.256	1308	1311	1314	rVB2	677	401	0.04%	0.006%
20	5.474	1374	1379	1382	rBV4	462	426	0.05%	0.006%
21	5.539	1387	1399	1424	rBV	263343	551204	59.14%	7.718%
22	5.992	1527	1540	1559	rBV	206114	430225	46.16%	6.024%
23	6.259	1621	1623	1626	rVB3	428	192	0.02%	0.003%
24	6.278	1628	1629	1634	rBV4	384	212	0.02%	0.003%
25	6.333	1640	1646	1649	rBV5	794	812	0.09%	0.011%
26	6.368	1653	1657	1660	rBV3	578	589	0.06%	0.008%
27	6.420	1670	1673	1674	rBV3	454	187	0.02%	0.003%
28	6.429	1674	1676	1680	rVB3	252	176	0.02%	0.002%
29	6.519	1703	1704	1708	rBV3	268	175	0.02%	0.002%
30	6.542	1708	1711	1715	rVB3	479	349	0.04%	0.005%
31	6.564	1715	1718	1724	rBV3	451	394	0.04%	0.006%
32	6.593	1724	1727	1728	rBV2	460	243	0.03%	0.003%
33	6.625	1734	1737	1742	rBV4	703	645	0.07%	0.009%
34	6.693	1754	1758	1760	rBV2	447	319	0.03%	0.004%
35	6.773	1781	1783	1785	rBV2	447	234	0.03%	0.003%
36	6.793	1785	1789	1792	rBV2	355	314	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031983.D
 Acq On : 08 Sep 2023 16:09
 Operator : SY/MD
 Sample : VIBLK229
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.831	1798	1801	1802	rBV	356	175	0.02%	0.002%
38	6.918	1814	1828	1862	rBV	116643	231915	24.88%	3.247%
39	7.249	1919	1931	1960	rBV	388307	705638	75.71%	9.880%
40	7.558	2017	2027	2059	rBV	81183	154373	16.56%	2.162%
41	7.786	2096	2098	2100	rBV2	643	384	0.04%	0.005%
42	7.834	2112	2113	2116	rBV2	491	175	0.02%	0.002%
43	7.854	2116	2119	2120	rBV3	387	214	0.02%	0.003%
44	7.982	2153	2159	2160	rVV4	697	641	0.07%	0.009%
45	8.031	2164	2174	2208	rBV	262291	493013	52.89%	6.903%
46	8.365	2272	2278	2294	rVB3	10540	18418	1.98%	0.258%
47	8.567	2339	2341	2343	rBV2	364	192	0.02%	0.003%
48	8.638	2359	2363	2365	rBV4	454	393	0.04%	0.006%
49	8.680	2372	2376	2378	rVB	455	262	0.03%	0.004%
50	8.703	2380	2383	2386	rVB3	654	366	0.04%	0.005%
51	8.719	2386	2388	2390	rBV	308	159	0.02%	0.002%
52	8.789	2399	2410	2444	rBV	406497	685543	73.55%	9.599%
53	9.011	2477	2479	2480	rBV	515	212	0.02%	0.003%
54	9.040	2483	2488	2491	rBV4	283	252	0.03%	0.004%
55	9.066	2492	2496	2498	rBV3	410	314	0.03%	0.004%
56	9.140	2516	2519	2521	rBV3	401	289	0.03%	0.004%
57	9.172	2526	2529	2532	rBV2	504	379	0.04%	0.005%
58	9.223	2542	2545	2547	rBV2	498	276	0.03%	0.004%
59	9.420	2604	2606	2609	rVB	416	162	0.02%	0.002%
60	9.445	2609	2614	2617	rVB4	636	551	0.06%	0.008%
61	9.468	2617	2621	2623	rBV2	428	320	0.03%	0.004%
62	9.500	2626	2631	2637	rBV5	722	854	0.09%	0.012%
63	9.555	2645	2648	2651	rBV3	383	304	0.03%	0.004%
64	9.645	2669	2676	2678	rBV4	674	709	0.08%	0.010%
65	9.680	2683	2687	2690	rBV3	374	356	0.04%	0.005%
66	9.754	2706	2710	2716	rVB3	407	437	0.05%	0.006%
67	9.857	2740	2742	2746	rVB4	453	229	0.02%	0.003%
68	9.879	2746	2749	2751	rBV2	407	232	0.02%	0.003%
69	10.027	2793	2795	2798	rBV2	565	340	0.04%	0.005%
70	10.114	2817	2822	2823	rBV2	471	388	0.04%	0.005%
71	10.159	2824	2836	2857	rVV	280467	458054	49.14%	6.414%
72	10.603	2971	2974	2976	rBV2	345	220	0.02%	0.003%
73	10.619	2976	2979	2982	rVV3	411	307	0.03%	0.004%
74	10.632	2982	2983	2991	rVB3	590	389	0.04%	0.005%
75	10.706	3004	3006	3010	rBV3	325	231	0.02%	0.003%
76	10.809	3036	3038	3041	rBV2	345	184	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031983.D
 Acq On : 08 Sep 2023 16:09
 Operator : SY/MD
 Sample : VIBLK229
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.956	3079	3084	3087	rBV4	517	523	0.06%	0.007%
78	11.027	3104	3106	3109	rBV2	512	402	0.04%	0.006%
79	11.143	3138	3142	3143	rBV2	537	364	0.04%	0.005%
80	11.188	3145	3156	3177	rVV	447624	696463	74.72%	9.752%
81	11.365	3208	3211	3216	rVB4	469	365	0.04%	0.005%
82	11.436	3230	3233	3234	rBV	426	173	0.02%	0.002%
83	11.516	3254	3258	3260	rBV3	741	655	0.07%	0.009%
84	11.564	3262	3273	3294	rVB	402745	641436	68.82%	8.982%
85	11.828	3353	3355	3359	rVB3	392	197	0.02%	0.003%
86	11.866	3364	3367	3370	rBV2	672	420	0.05%	0.006%
87	12.011	3408	3412	3414	rBV2	602	463	0.05%	0.006%
88	12.300	3498	3502	3505	rBV5	424	438	0.05%	0.006%
89	12.513	3566	3568	3569	rBV	404	160	0.02%	0.002%
90	12.571	3583	3586	3589	rBV3	507	406	0.04%	0.006%
91	12.728	3633	3635	3636	rBV2	316	163	0.02%	0.002%
92	12.837	3667	3669	3674	rVB3	1163	651	0.07%	0.009%
93	12.892	3681	3686	3689	rVB4	803	835	0.09%	0.012%
94	12.908	3689	3691	3695	rBV3	493	450	0.05%	0.006%
95	13.114	3753	3755	3757	rVB	711	227	0.02%	0.003%
96	13.127	3757	3759	3761	rBV2	472	244	0.03%	0.003%
97	13.297	3806	3812	3814	rBV2	485	589	0.06%	0.008%
98	13.497	3872	3874	3876	rBV3	534	256	0.03%	0.004%
99	13.683	3928	3932	3934	rBV2	895	665	0.07%	0.009%
100	13.950	4013	4015	4018	rBV3	501	412	0.04%	0.006%




Sum of corrected areas: 7141735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031983.D
Acq On : 08 Sep 2023 16:09
Operator : SY/MD
Sample : VIBLK229
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

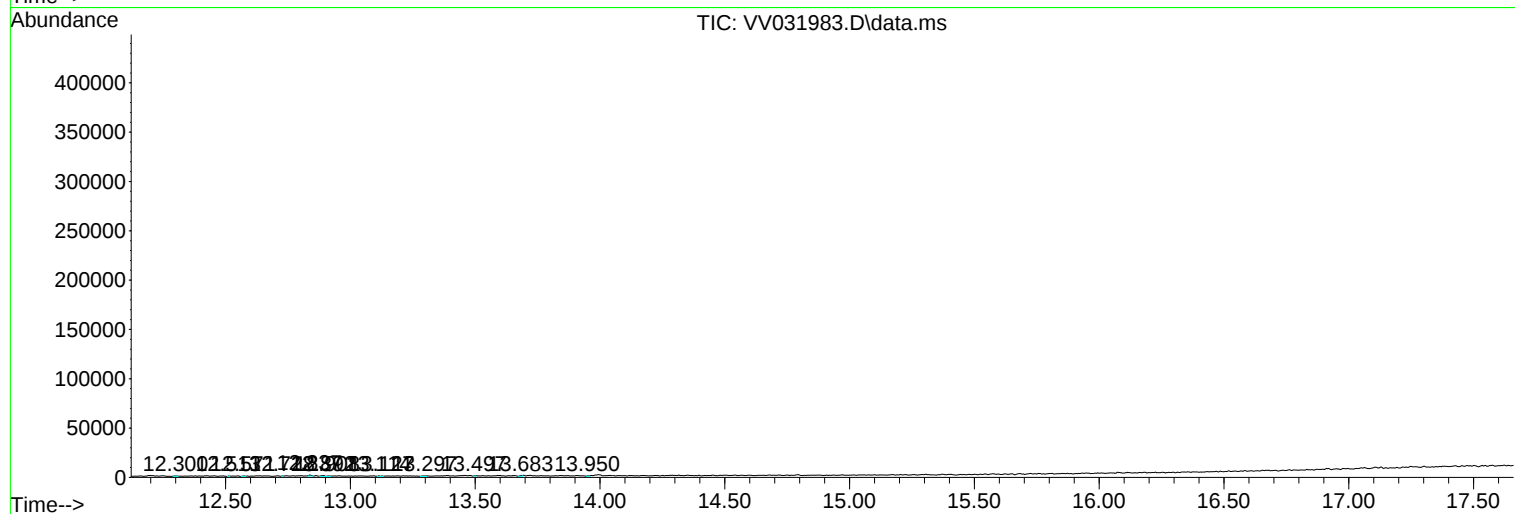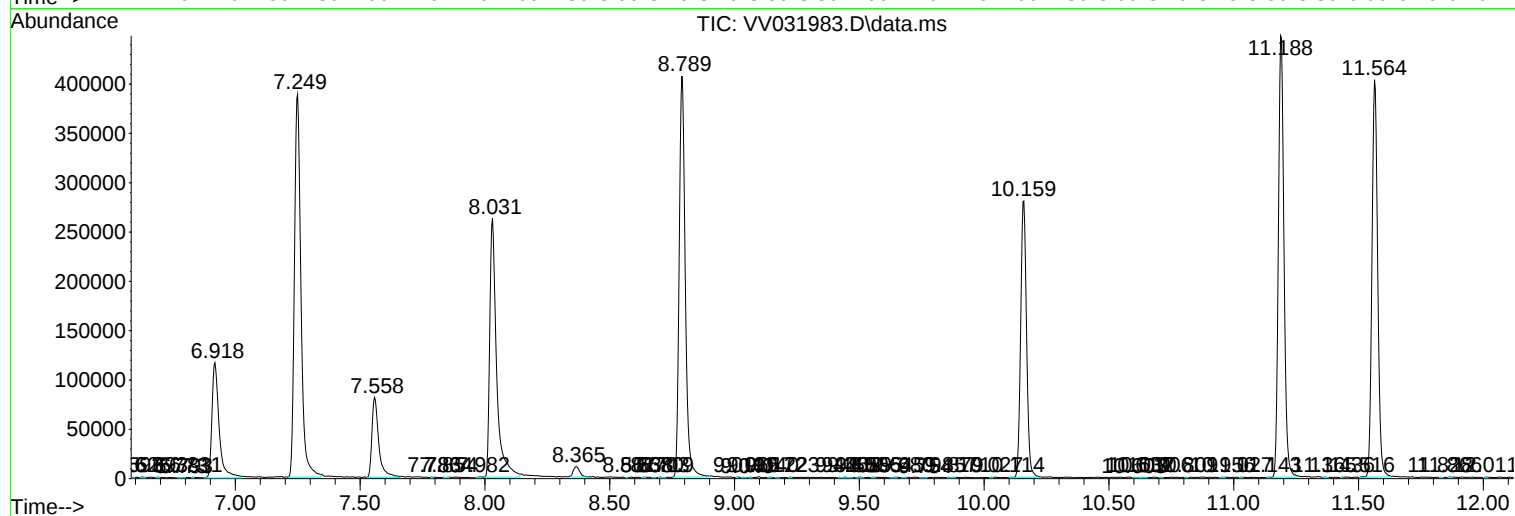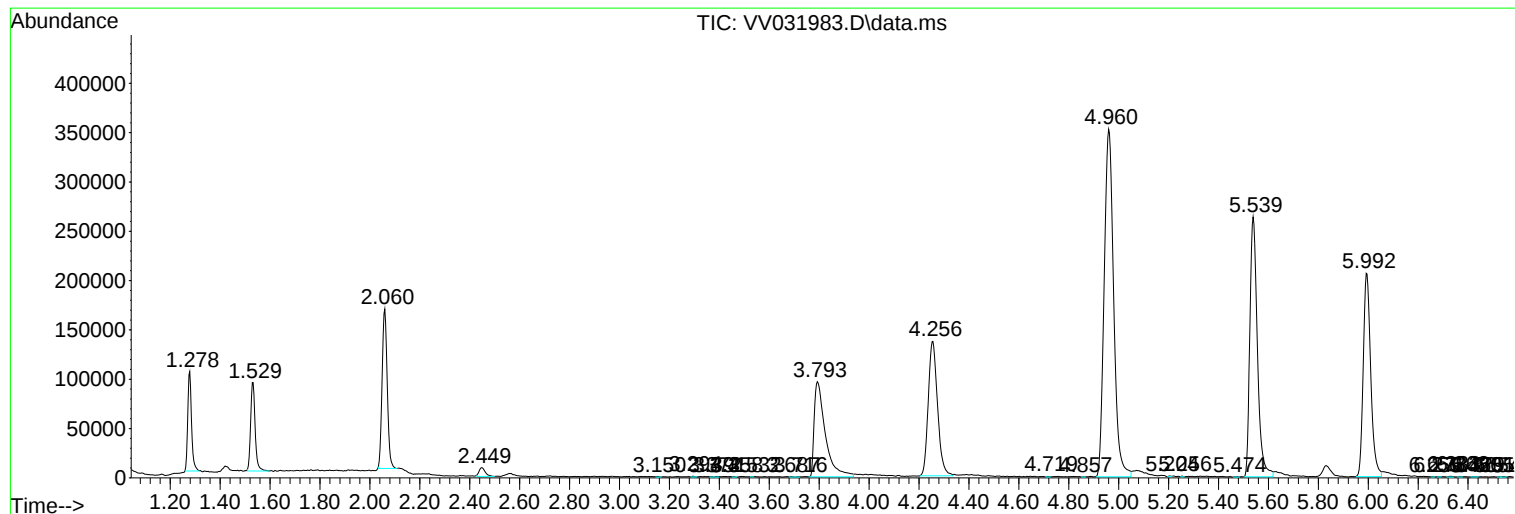

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031983.D
Acq On : 08 Sep 2023 16:09
Operator : SY/MD
Sample : VIBLK229
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031983.D
Acq On : 08 Sep 2023 16:09
Operator : SY/MD
Sample : VIBLK229
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
