

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031984.D
 Acq On : 08 Sep 2023 16:35
 Operator : SY/MD
 Sample : 04280-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	114622	122428	13.34%	1.625%
2	1.529	146	152	166	rVB	93106	112346	12.24%	1.491%
3	2.060	308	317	334	rVB	184022	266255	29.02%	3.533%
4	2.677	505	509	511	rBV2	405	305	0.03%	0.004%
5	2.857	561	565	569	rBV4	479	528	0.06%	0.007%
6	2.934	587	589	593	rBV4	460	312	0.03%	0.004%
7	3.105	637	642	648	rVV5	508	708	0.08%	0.009%
8	3.230	677	681	685	rBV3	446	538	0.06%	0.007%
9	3.461	751	753	756	rVB3	324	195	0.02%	0.003%
10	3.497	761	764	766	rBV	332	193	0.02%	0.003%
11	3.609	796	799	802	rBV3	397	293	0.03%	0.004%
12	3.748	839	842	844	rBV2	417	281	0.03%	0.004%
13	3.793	844	856	891	rBV	80327	234082	25.51%	3.106%
14	4.252	983	999	1027	rBV	135356	350503	38.20%	4.651%
15	4.548	1088	1091	1093	rBV4	568	312	0.03%	0.004%
16	4.693	1133	1136	1139	rBV3	433	403	0.04%	0.005%
17	4.789	1163	1166	1170	rBV3	368	257	0.03%	0.003%
18	4.815	1173	1174	1178	rVB3	497	236	0.03%	0.003%
19	4.841	1180	1182	1185	rBV4	401	183	0.02%	0.002%
20	4.879	1192	1194	1198	rVB2	490	247	0.03%	0.003%
21	4.960	1203	1219	1244	rBV2	351180	917577	100.00%	12.176%
22	5.256	1309	1311	1314	rBV3	559	383	0.04%	0.005%
23	5.294	1321	1323	1327	rBV3	865	689	0.08%	0.009%
24	5.407	1355	1358	1361	rBV3	433	268	0.03%	0.004%
25	5.471	1374	1378	1380	rBV4	662	478	0.05%	0.006%
26	5.539	1386	1399	1421	rBV	326732	669652	72.98%	8.886%
27	5.770	1469	1471	1474	rVB2	742	301	0.03%	0.004%
28	5.786	1474	1476	1479	rVB2	668	375	0.04%	0.005%
29	5.834	1479	1491	1506	rBV2	10900	24762	2.70%	0.329%
30	5.947	1524	1526	1527	rBV2	482	176	0.02%	0.002%
31	5.992	1528	1540	1564	rVV	200493	419117	45.68%	5.562%
32	6.326	1639	1644	1647	rBV3	659	592	0.06%	0.008%
33	6.394	1662	1665	1668	rVB3	442	307	0.03%	0.004%
34	6.416	1668	1672	1675	rBV	283	265	0.03%	0.004%
35	6.500	1692	1698	1704	rBV4	463	677	0.07%	0.009%
36	6.542	1709	1711	1714	rBV	297	218	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031984.D
 Acq On : 08 Sep 2023 16:35
 Operator : SY/MD
 Sample : 04280-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.603	1725	1730	1732	rBV4	591	519	0.06%	0.007%
38	6.744	1770	1774	1775	rBV2	293	217	0.02%	0.003%
39	6.754	1775	1777	1783	rVB5	425	298	0.03%	0.004%
40	6.831	1797	1801	1805	rBV3	344	330	0.04%	0.004%
41	6.918	1812	1828	1859	rBV	115219	228360	24.89%	3.030%
42	7.098	1882	1884	1890	rBV2	468	284	0.03%	0.004%
43	7.124	1890	1892	1894	rBV2	438	220	0.02%	0.003%
44	7.246	1919	1930	1965	rBV	409578	746172	81.32%	9.902%
45	7.558	2016	2027	2047	rBV	82008	149030	16.24%	1.978%
46	7.825	2108	2110	2112	rBV3	392	202	0.02%	0.003%
47	7.860	2119	2121	2124	rBV3	450	349	0.04%	0.005%
48	7.918	2135	2139	2142	rBV2	439	351	0.04%	0.005%
49	7.944	2145	2147	2151	rBV	425	265	0.03%	0.004%
50	8.030	2164	2174	2206	rBV	230311	444264	48.42%	5.895%
51	8.506	2320	2322	2325	rBV4	415	222	0.02%	0.003%
52	8.577	2341	2344	2349	rBV3	502	443	0.05%	0.006%
53	8.789	2398	2410	2437	rBV	495900	836618	91.18%	11.102%
54	9.008	2476	2478	2482	rVB3	806	514	0.06%	0.007%
55	9.037	2483	2487	2491	rVB6	679	607	0.07%	0.008%
56	9.059	2491	2494	2495	rBV	501	193	0.02%	0.003%
57	9.243	2550	2551	2554	rVB	365	179	0.02%	0.002%
58	9.268	2557	2559	2561	rBV3	360	190	0.02%	0.003%
59	9.320	2572	2575	2578	rBV3	388	326	0.04%	0.004%
60	9.358	2586	2587	2590	rBV2	390	218	0.02%	0.003%
61	9.442	2609	2613	2615	rBV	420	246	0.03%	0.003%
62	9.455	2615	2617	2621	rVV3	387	205	0.02%	0.003%
63	9.509	2625	2634	2638	rVB6	602	759	0.08%	0.010%
64	9.535	2638	2642	2646	rBV3	714	651	0.07%	0.009%
65	9.574	2651	2654	2656	rBV2	425	325	0.04%	0.004%
66	9.854	2737	2741	2743	rBV2	584	372	0.04%	0.005%
67	9.876	2744	2748	2754	rVV5	574	716	0.08%	0.010%
68	9.921	2759	2762	2765	rBV2	462	310	0.03%	0.004%
69	9.947	2768	2770	2774	rBV3	338	224	0.02%	0.003%
70	9.998	2783	2786	2790	rVB3	702	530	0.06%	0.007%
71	10.021	2790	2793	2796	rBV3	340	276	0.03%	0.004%
72	10.156	2824	2835	2865	rVB	262182	424577	46.27%	5.634%
73	10.374	2901	2903	2908	rVB2	530	378	0.04%	0.005%
74	10.481	2934	2936	2943	rVB4	663	589	0.06%	0.008%
75	10.513	2943	2946	2947	rBV2	321	186	0.02%	0.002%
76	10.619	2975	2979	2984	rVB3	677	686	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031984.D
 Acq On : 08 Sep 2023 16:35
 Operator : SY/MD
 Sample : 04280-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.644	2984	2987	2989	rBV2	296	212	0.02%	0.003%
78	10.712	3003	3008	3011	rBV4	663	657	0.07%	0.009%
79	10.735	3011	3015	3020	rVV3	469	529	0.06%	0.007%
80	10.812	3037	3039	3044	rBV2	347	329	0.04%	0.004%
81	10.853	3050	3052	3056	rBV	347	257	0.03%	0.003%
82	10.889	3060	3063	3065	rBV2	375	236	0.03%	0.003%
83	10.934	3073	3077	3080	rBV3	581	414	0.05%	0.005%
84	10.982	3089	3092	3100	rVB5	638	569	0.06%	0.008%
85	11.072	3113	3120	3122	rBV3	504	463	0.05%	0.006%
86	11.117	3132	3134	3137	rVB3	552	266	0.03%	0.004%
87	11.136	3137	3140	3142	rBV3	440	332	0.04%	0.004%
88	11.188	3145	3156	3175	rBV	562281	886661	96.63%	11.766%
89	11.403	3221	3223	3225	rBV3	384	173	0.02%	0.002%
90	11.564	3262	3273	3294	rBV	429366	673091	73.36%	8.932%
91	11.966	3397	3398	3401	rVB2	542	243	0.03%	0.003%
92	11.988	3401	3405	3408	rBV5	566	536	0.06%	0.007%
93	12.033	3417	3419	3421	rBV2	557	277	0.03%	0.004%
94	12.233	3478	3481	3486	rBV4	462	500	0.05%	0.007%
95	12.371	3522	3524	3527	rBV3	579	301	0.03%	0.004%
96	12.435	3541	3544	3549	rBV4	390	378	0.04%	0.005%
97	12.960	3705	3707	3710	rBV2	475	306	0.03%	0.004%
98	13.615	3909	3911	3915	rBV3	744	511	0.06%	0.007%
99	13.686	3931	3933	3935	rBV	640	319	0.03%	0.004%
100	13.863	3985	3988	3989	rBV3	617	319	0.03%	0.004%




Sum of corrected areas: 7535722

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031984.D
Acq On : 08 Sep 2023 16:35
Operator : SY/MD
Sample : 04280-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

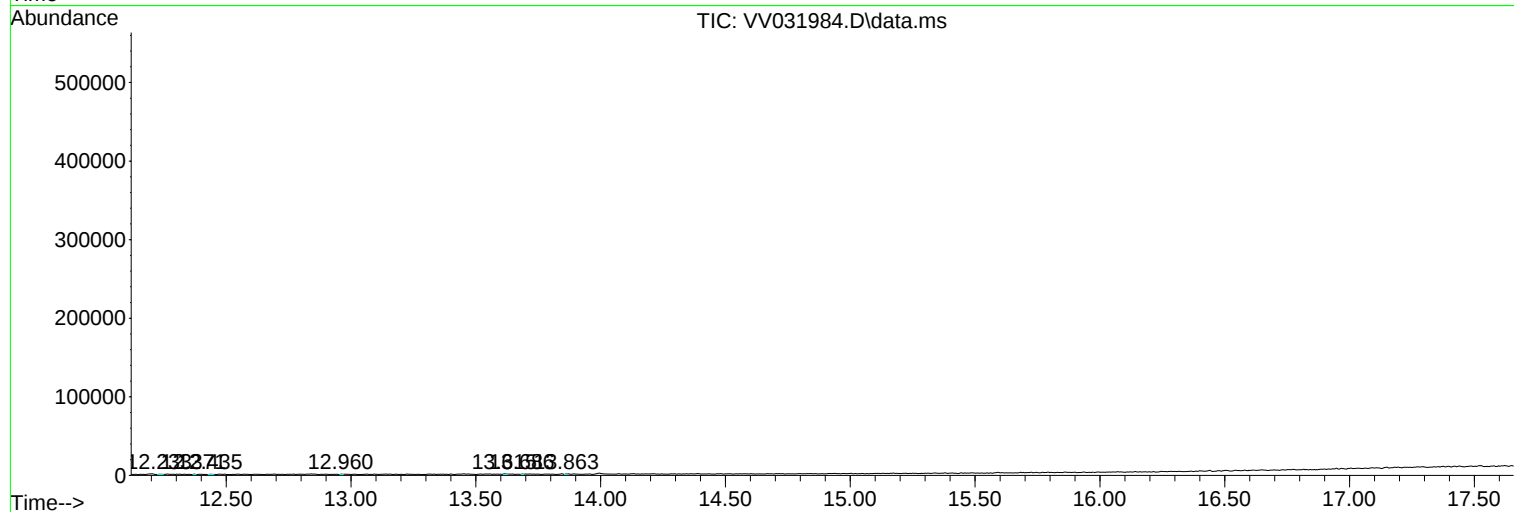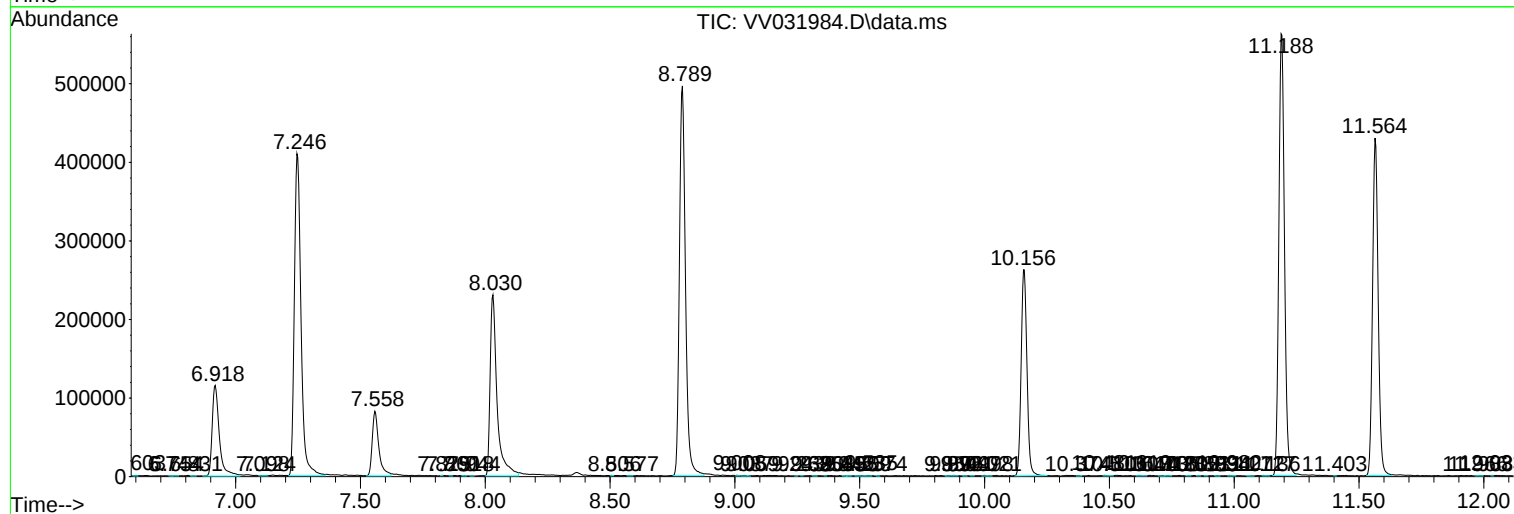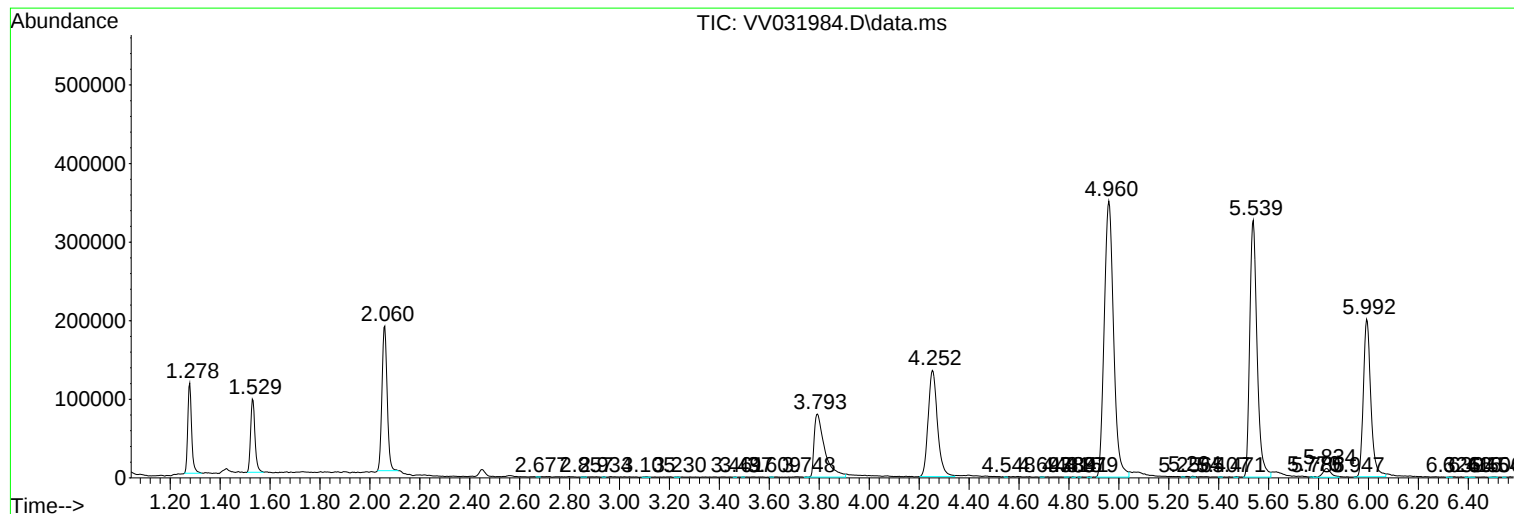

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031984.D
Acq On : 08 Sep 2023 16:35
Operator : SY/MD
Sample : 04280-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031984.D
Acq On : 08 Sep 2023 16:35
Operator : SY/MD
Sample : 04280-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------