

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031985.D
 Acq On : 08 Sep 2023 17:00
 Operator : SY/MD
 Sample : 04277-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	108504	115599	13.11%	1.585%
2	1.529	146	152	166	rVB	89525	109164	12.38%	1.496%
3	2.060	309	317	332	rVB	175015	253414	28.75%	3.474%
4	2.449	431	438	447	rVB	8073	12603	1.43%	0.173%
5	2.825	552	555	558	rVB3	677	324	0.04%	0.004%
6	3.024	614	617	619	rBV2	347	179	0.02%	0.002%
7	3.044	619	623	624	rBV2	335	230	0.03%	0.003%
8	3.079	632	634	636	rBV2	412	176	0.02%	0.002%
9	3.172	661	663	665	rBV2	554	307	0.03%	0.004%
10	3.391	729	731	735	rVB3	385	232	0.03%	0.003%
11	3.417	736	739	743	rVB4	551	397	0.05%	0.005%
12	3.516	766	770	773	rBV	554	440	0.05%	0.006%
13	3.584	788	791	793	rBV2	335	176	0.02%	0.002%
14	3.600	795	796	797	rBV2	255	62	0.01%	0.001%
15	3.648	808	811	814	rBV3	498	419	0.05%	0.006%
16	3.712	828	831	833	rVB	414	193	0.02%	0.003%
17	3.725	833	835	837	rBV	329	164	0.02%	0.002%
18	3.741	837	840	841	rBV	426	213	0.02%	0.003%
19	3.751	841	843	845	rVB2	372	133	0.02%	0.002%
20	3.793	846	856	892	rBV	80812	237838	26.98%	3.260%
21	4.253	985	999	1026	rBV	129523	326782	37.07%	4.479%
22	4.558	1091	1094	1096	rBV4	566	388	0.04%	0.005%
23	4.802	1169	1170	1172	rBV	406	172	0.02%	0.002%
24	4.883	1191	1195	1202	rBV3	544	675	0.08%	0.009%
25	4.960	1202	1219	1243	rBV2	339674	881494	100.00%	12.083%
26	5.449	1367	1371	1374	rBV5	516	427	0.05%	0.006%
27	5.471	1374	1378	1380	rVB4	503	326	0.04%	0.004%
28	5.535	1387	1398	1420	rBV	307256	637210	72.29%	8.735%
29	5.831	1480	1490	1507	rBV5	10604	22128	2.51%	0.303%
30	5.992	1527	1540	1563	rBV	193921	409707	46.48%	5.616%
31	6.436	1675	1678	1681	rVB3	383	180	0.02%	0.002%
32	6.455	1682	1684	1687	rBV	299	139	0.02%	0.002%
33	6.542	1709	1711	1713	rBV2	212	130	0.01%	0.002%
34	6.664	1746	1749	1754	rBV5	461	543	0.06%	0.007%
35	6.728	1765	1769	1772	rBV3	701	633	0.07%	0.009%
36	6.812	1790	1795	1799	rBV4	639	636	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031985.D
 Acq On : 08 Sep 2023 17:00
 Operator : SY/MD
 Sample : 04277-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.918	1817	1828	1861	rBV	113193	220464	25.01%	3.022%
38	7.246	1918	1930	1967	rBV	396623	720137	81.70%	9.871%
39	7.558	2017	2027	2054	rBV	78510	145075	16.46%	1.989%
40	7.799	2098	2102	2107	rBV3	542	577	0.07%	0.008%
41	7.831	2107	2112	2115	rBV3	518	467	0.05%	0.006%
42	7.867	2119	2123	2125	rBV2	629	410	0.05%	0.006%
43	7.928	2137	2142	2143	rBV3	545	411	0.05%	0.006%
44	7.979	2155	2158	2160	rBV2	563	331	0.04%	0.005%
45	8.030	2164	2174	2209	rBV	229849	445712	50.56%	6.110%
46	8.362	2269	2277	2294	rVB4	4372	8529	0.97%	0.117%
47	8.429	2296	2298	2301	rBV2	612	307	0.03%	0.004%
48	8.519	2322	2326	2327	rBV	495	233	0.03%	0.003%
49	8.529	2327	2329	2331	rVB	420	181	0.02%	0.002%
50	8.545	2331	2334	2336	rBV2	649	463	0.05%	0.006%
51	8.609	2351	2354	2358	rBV4	487	398	0.05%	0.005%
52	8.789	2398	2410	2433	rBV	481304	801241	90.90%	10.983%
53	9.082	2499	2501	2506	rBV3	586	327	0.04%	0.004%
54	9.130	2515	2516	2518	rBV2	304	111	0.01%	0.002%
55	9.233	2546	2548	2550	rBV2	281	129	0.01%	0.002%
56	9.262	2555	2557	2559	rVV2	285	130	0.01%	0.002%
57	9.329	2575	2578	2580	rBV2	475	233	0.03%	0.003%
58	9.439	2606	2612	2616	rBV4	692	671	0.08%	0.009%
59	9.465	2617	2620	2622	rVV2	449	219	0.02%	0.003%
60	9.538	2638	2643	2644	rBV2	562	349	0.04%	0.005%
61	9.603	2660	2663	2665	rBV3	365	239	0.03%	0.003%
62	9.670	2681	2684	2686	rBV2	299	199	0.02%	0.003%
63	9.722	2698	2700	2702	rVB	283	113	0.01%	0.002%
64	9.738	2702	2705	2710	rVB2	461	410	0.05%	0.006%
65	9.834	2732	2735	2736	rBV2	457	311	0.04%	0.004%
66	10.066	2804	2807	2809	rBV2	392	268	0.03%	0.004%
67	10.156	2823	2835	2854	rBV	256871	419295	47.57%	5.748%
68	10.265	2867	2869	2872	rBV2	594	394	0.04%	0.005%
69	10.352	2894	2896	2899	rVB2	432	194	0.02%	0.003%
70	10.368	2899	2901	2905	rBV2	305	216	0.02%	0.003%
71	10.391	2905	2908	2912	rVV3	375	336	0.04%	0.005%
72	10.564	2960	2962	2963	rBV3	252	111	0.01%	0.002%
73	10.764	3022	3024	3026	rBV2	446	250	0.03%	0.003%
74	10.960	3083	3085	3089	rVB3	306	213	0.02%	0.003%
75	10.995	3089	3096	3097	rBV3	434	461	0.05%	0.006%
76	11.117	3129	3134	3137	rBV4	540	384	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
 Data File : VV031985.D
 Acq On : 08 Sep 2023 17:00
 Operator : SY/MD
 Sample : 04277-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

77	11.133	3137	3139	3142	rBV2	361	199	0.02%	0.003%
78	11.188	3145	3156	3177	rBV	545710	850204	96.45%	11.654%
79	11.448	3235	3237	3241	rVB2	403	245	0.03%	0.003%
80	11.471	3242	3244	3245	rBV2	397	193	0.02%	0.003%
81	11.564	3261	3273	3294	rBV	410194	658124	74.66%	9.021%
82	11.860	3363	3365	3366	rBV	295	116	0.01%	0.002%
83	11.899	3372	3377	3378	rBV2	460	379	0.04%	0.005%
84	12.085	3433	3435	3437	rBV2	465	283	0.03%	0.004%
85	12.275	3492	3494	3497	rVB2	440	214	0.02%	0.003%
86	12.304	3501	3503	3504	rBV	287	134	0.02%	0.002%
87	12.985	3712	3715	3717	rBV2	281	138	0.02%	0.002%
88	13.281	3804	3807	3810	rVB	652	360	0.04%	0.005%
89	13.535	3884	3886	3892	rBV2	431	335	0.04%	0.005%




Sum of corrected areas: 7295256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031985.D
Acq On : 08 Sep 2023 17:00
Operator : SY/MD
Sample : 04277-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

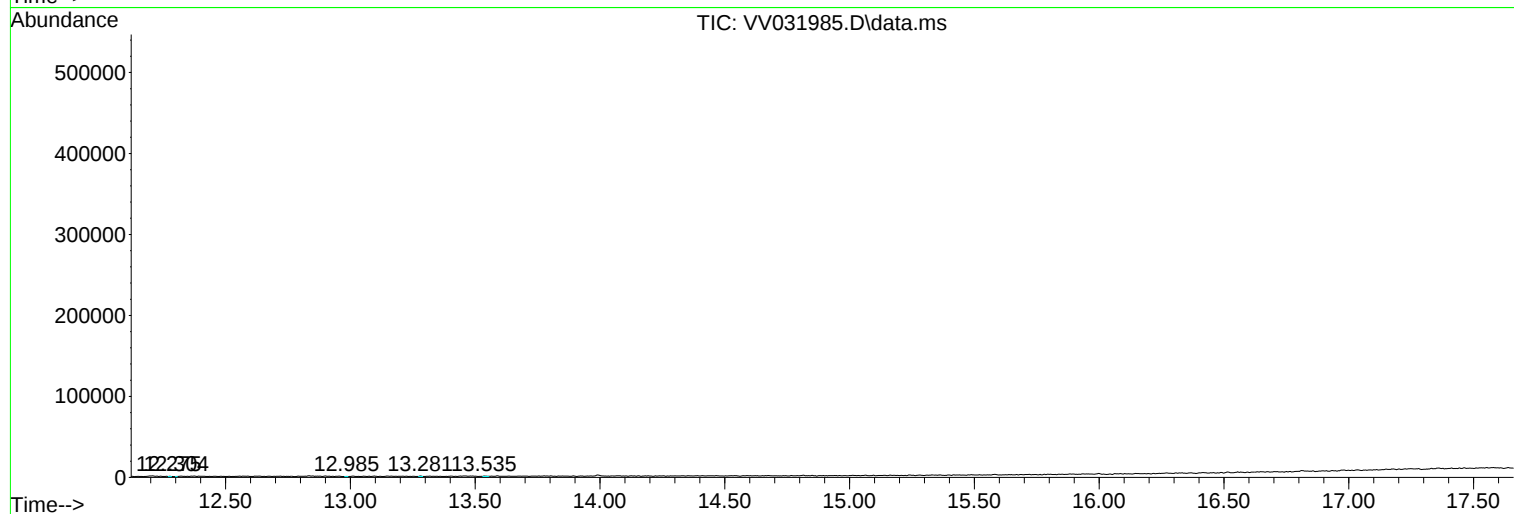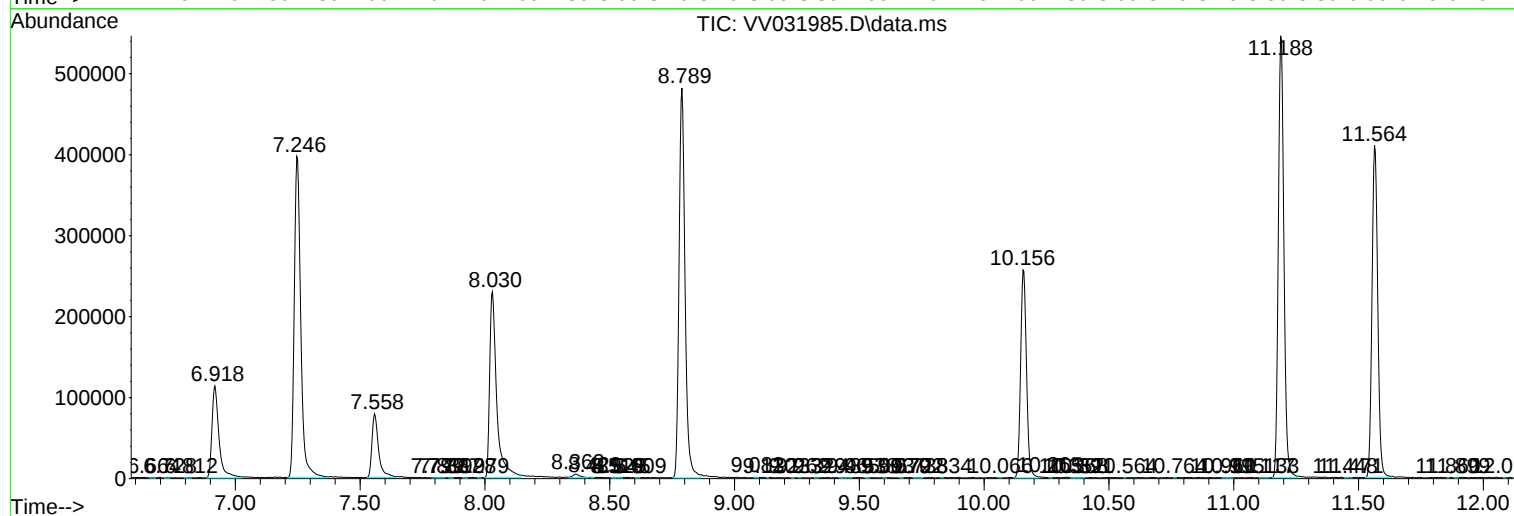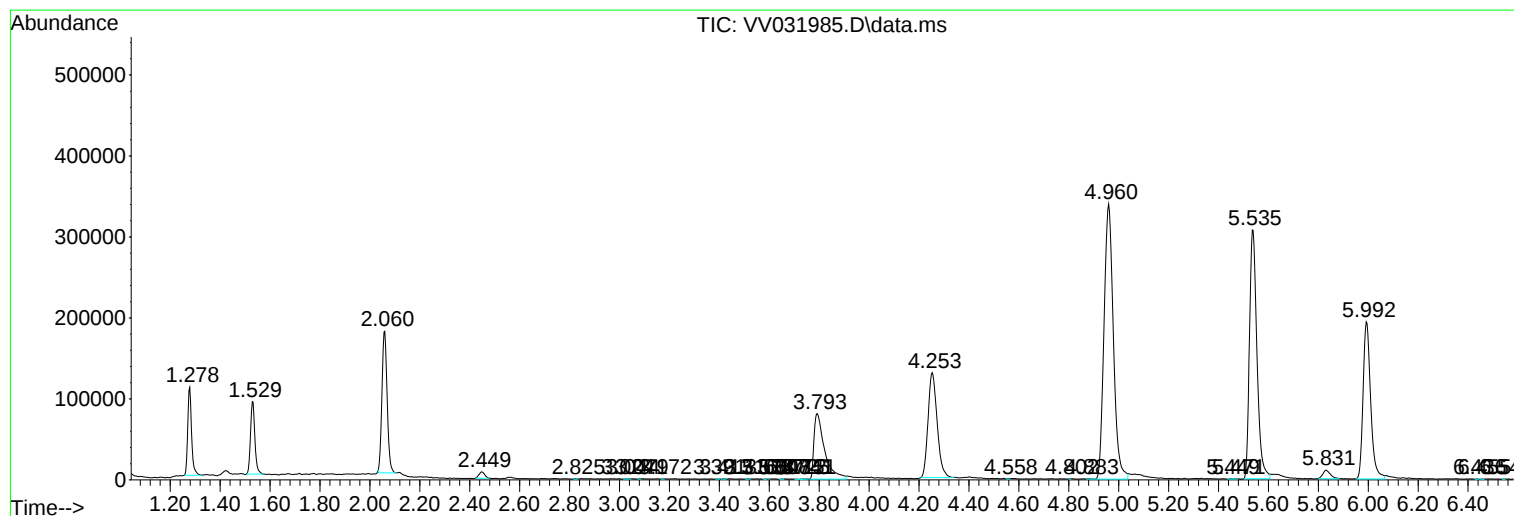

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031985.D
Acq On : 08 Sep 2023 17:00
Operator : SY/MD
Sample : 04277-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031985.D
Acq On : 08 Sep 2023 17:00
Operator : SY/MD
Sample : 04277-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
