
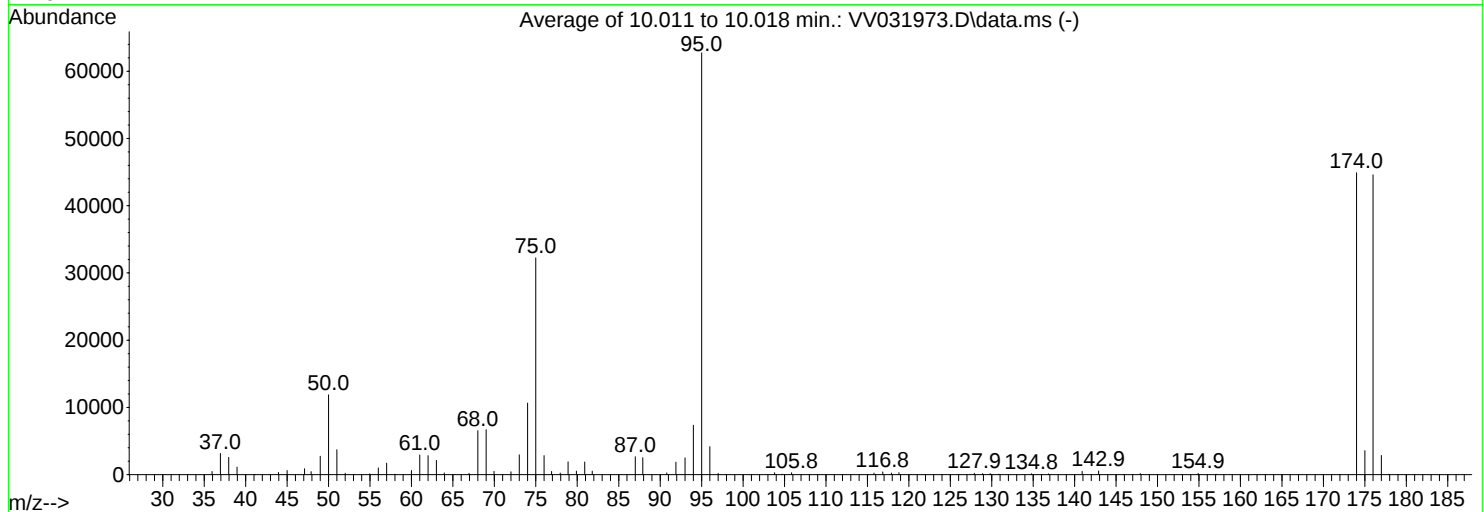


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090823\
Data File : VV031973.D
Acq On : 08 Sep 2023 09:13
Operator : SY/MD
Sample : BFB209
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB209

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Sat Sep 09 05:33:49 2023

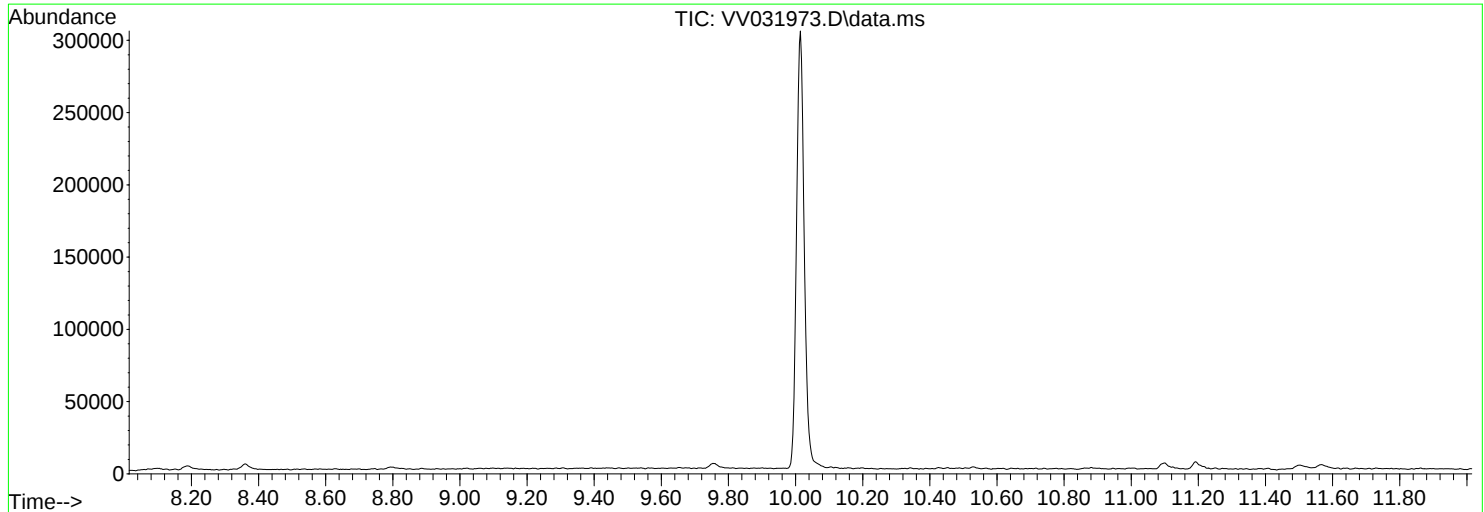

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	11885	PASS
75	95	30	80	51.4	32248	PASS
95	95	100	100	100.0	62733	PASS
96	95	5	9	6.7	4178	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.6	44901	PASS
175	174	5	9	7.9	3567	PASS
176	174	95	105	99.3	44605	PASS
177	176	5	10	6.4	2858	PASS

m/z	Abundance
36.00	1596.0
36.90	178.0
37.90	585.0
39.00	122.0
39.90	216.0
41.00	220.0
41.80	130.0
43.10	124.0
43.90	390.0
55.10	139.0
77.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
35.90	2000.0
37.00	3507.0
38.00	3190.0
38.90	1152.0
39.90	236.0
40.90	166.0
42.00	122.0
42.90	173.0
44.00	676.0
45.00	620.0
47.10	944.0
47.90	443.0
49.00	2731.0
50.00	12336.0
51.00	3754.0
52.00	236.0
54.90	255.0
56.00	999.0
57.00	1829.0
60.00	671.0
61.00	3003.0
62.00	2906.0
63.00	2129.0
64.00	246.0
67.00	206.0
68.00	6767.0
69.00	6637.0
69.90	548.0
72.00	434.0
73.00	2998.0
74.00	10602.0
75.00	32792.0
76.00	2997.0
76.90	561.0
78.00	277.0
78.90	1904.0
79.90	530.0
80.90	1993.0
81.80	522.0
87.00	2782.0
87.90	2420.0
90.80	269.0
91.90	1704.0
93.00	2528.0
94.00	7548.0
95.00	63160.0
96.00	4345.0
97.00	186.0
103.80	312.0
104.70	104.0
105.90	308.0
115.80	209.0
116.90	480.0
117.90	281.0
118.80	335.0
127.90	210.0
128.90	173.0
129.70	189.0
134.80	147.0
136.80	119.0
140.90	474.0
142.90	579.0
147.90	151.0
154.90	190.0
157.00	126.0
171.90	111.0
174.00	44144.0
175.00	3692.0
176.00	43608.0
177.00	2858.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	2104.0
37.00	3406.0
38.00	3248.0
39.00	1317.0
39.90	215.0
40.80	154.0
41.20	151.0
42.00	104.0
42.90	166.0
44.00	739.0
45.00	643.0
47.10	938.0
47.90	477.0
49.00	2822.0
50.00	12202.0
51.00	3835.0
52.00	213.0
54.90	265.0
56.00	1035.0
57.00	1744.0
58.00	108.0
60.00	644.0
61.00	3006.0
62.00	2869.0
63.00	2186.0
63.90	264.0
66.90	192.0
68.00	6795.0
69.00	6960.0
70.00	515.0
72.00	438.0
73.00	3073.0
74.00	10963.0
75.00	33336.0
76.00	2911.0
76.90	616.0
77.90	244.0
78.90	1981.0
79.90	540.0
80.90	1937.0
81.80	550.0
87.00	2756.0
87.90	2651.0
90.80	278.0
91.90	1959.0
93.00	2555.0
94.00	7616.0
95.00	64672.0
96.00	4297.0
97.00	189.0
103.80	307.0
104.70	103.0
105.80	302.0
115.80	247.0
116.80	412.0
117.90	262.0
118.80	316.0
127.90	238.0
128.90	170.0
129.80	181.0
130.80	111.0
134.80	145.0
136.90	104.0
140.90	515.0
142.90	561.0
147.90	156.0
154.90	197.0
157.10	118.0
174.00	46336.0
175.00	3696.0
176.00	46008.0
177.00	2973.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	2151.0
37.00	3041.0
38.00	3043.0
39.00	1257.0
39.90	226.0
40.80	156.0
43.00	146.0
44.00	787.0
45.00	614.0
47.10	799.0
47.90	466.0
49.00	2680.0
50.00	11117.0
51.00	3543.0
52.00	171.0
54.90	277.0
56.00	969.0
57.00	1546.0
58.00	129.0
60.00	531.0
61.00	2756.0
62.00	2700.0
63.00	2025.0
63.90	248.0
66.90	178.0
68.00	6064.0
69.00	6495.0
70.00	474.0
72.00	409.0
73.00	2809.0
74.00	10323.0
75.00	30616.0
76.00	2594.0
76.90	604.0
77.90	210.0
78.90	1806.0
79.90	524.0
80.90	1729.0
81.80	487.0
87.00	2483.0
87.90	2532.0
90.80	267.0
91.90	1940.0
93.00	2436.0
94.00	6868.0
95.00	60368.0
96.00	3891.0
97.00	180.0
103.80	258.0
105.80	276.0
115.10	108.0
115.80	260.0
116.80	310.0
117.90	205.0
118.80	275.0
127.90	230.0
128.90	141.0
129.90	162.0
130.90	107.0
134.80	110.0
136.90	103.0
140.90	515.0
142.90	532.0
145.90	101.0
147.90	161.0
154.90	200.0
174.00	44224.0
175.00	3313.0
176.00	44200.0
177.00	2742.0
177.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209