



Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090919\
Data File : VV012645.D
Acq On : 10 Sep 2019 01:21
Operator : SY/MD
Sample : K4724-06
Misc : 25mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 10 09:36:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 10 09:27:53 2019
Response via : Initial Calibration

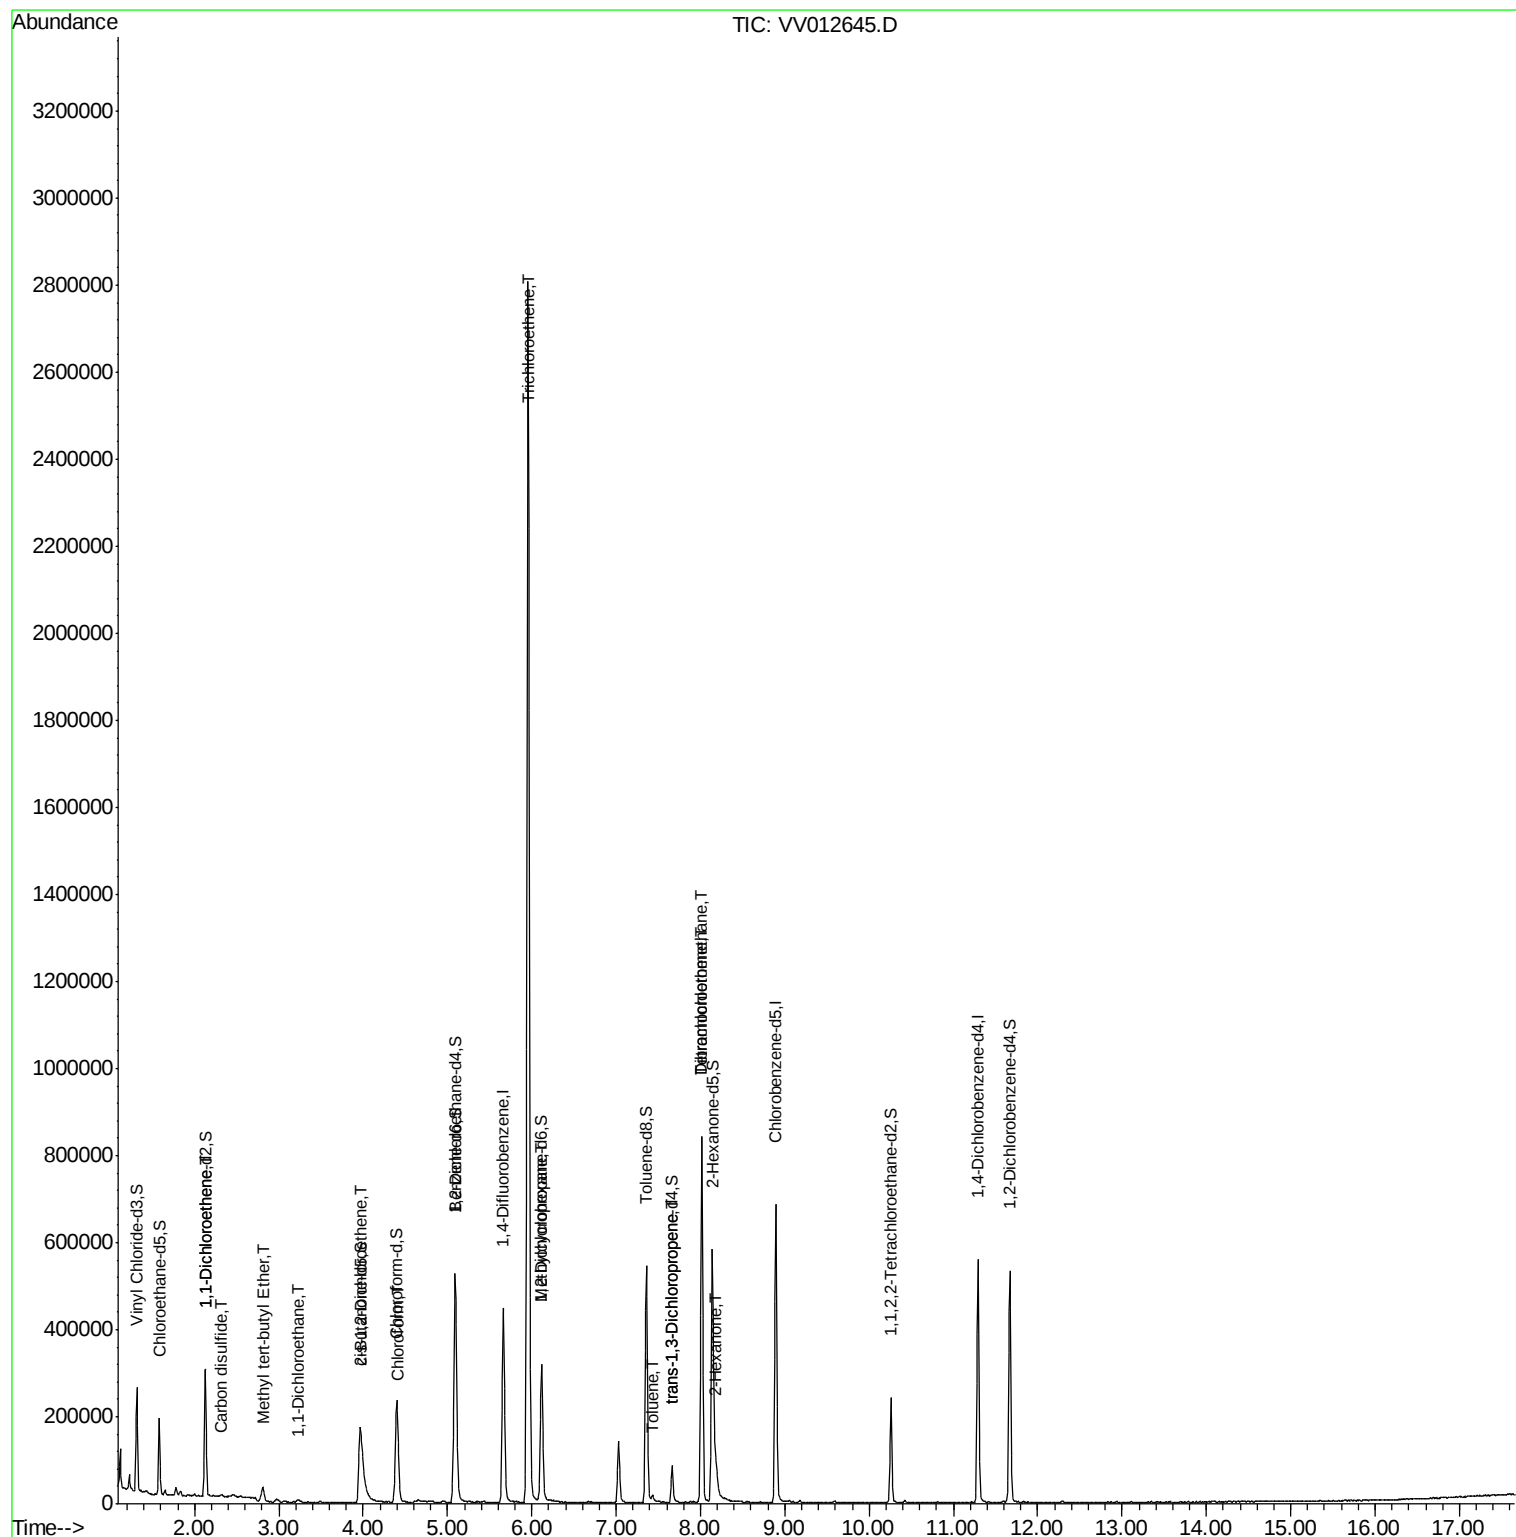

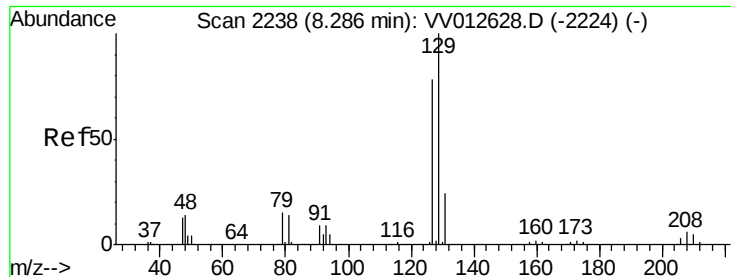

#49

Dibromochloromethane

Concen: 7.222 ug/L

RT: 8.02 min Scan# 2154

Delta R.T. -0.27 min

Lab File: VV012645.D

Acq: 10 Sep 2019 01:21

Instrument :
MSVOA_V
ClientSampleId :

Tot Ion:129 Resp: 166038

Ion Ratio Lower Upper

129 100

127 0.0 53.5 99.5#

