

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090919\
 Data File : VV012640.D
 Acq On : 09 Sep 2019 23:08
 Operator : SY/MD
 Sample : K4780-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0BM9

Quant Time: Sep 11 01:19:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 10 09:27:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	392818	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	391522	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	158566	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	122341	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.58	69	108004	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.00%
11) 1,1-Dichloroethene-d2	2.13	63	149258	3.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.40%
20) 2-Butanone-d5	3.93	46	367379	57.29	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.58%
24) Chloroform-d	4.40	84	227997	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.08	65	121542	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.10	84	446215	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.12	67	148503	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.36	98	353133	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	7.66	79	48507	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	8.13	63	197965	51.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.40%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	102349	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	148254	5.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.40%


Target Compounds				Ovalue
13) Acetone	2.19	43	6800	1.809 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090919\
Data File : VV012640.D
Acq On : 09 Sep 2019 23:08
Operator : SY/MD
Sample : K4780-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0BM9

Quant Time: Sep 11 01:19:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 10 09:27:53 2019
Response via : Initial Calibration

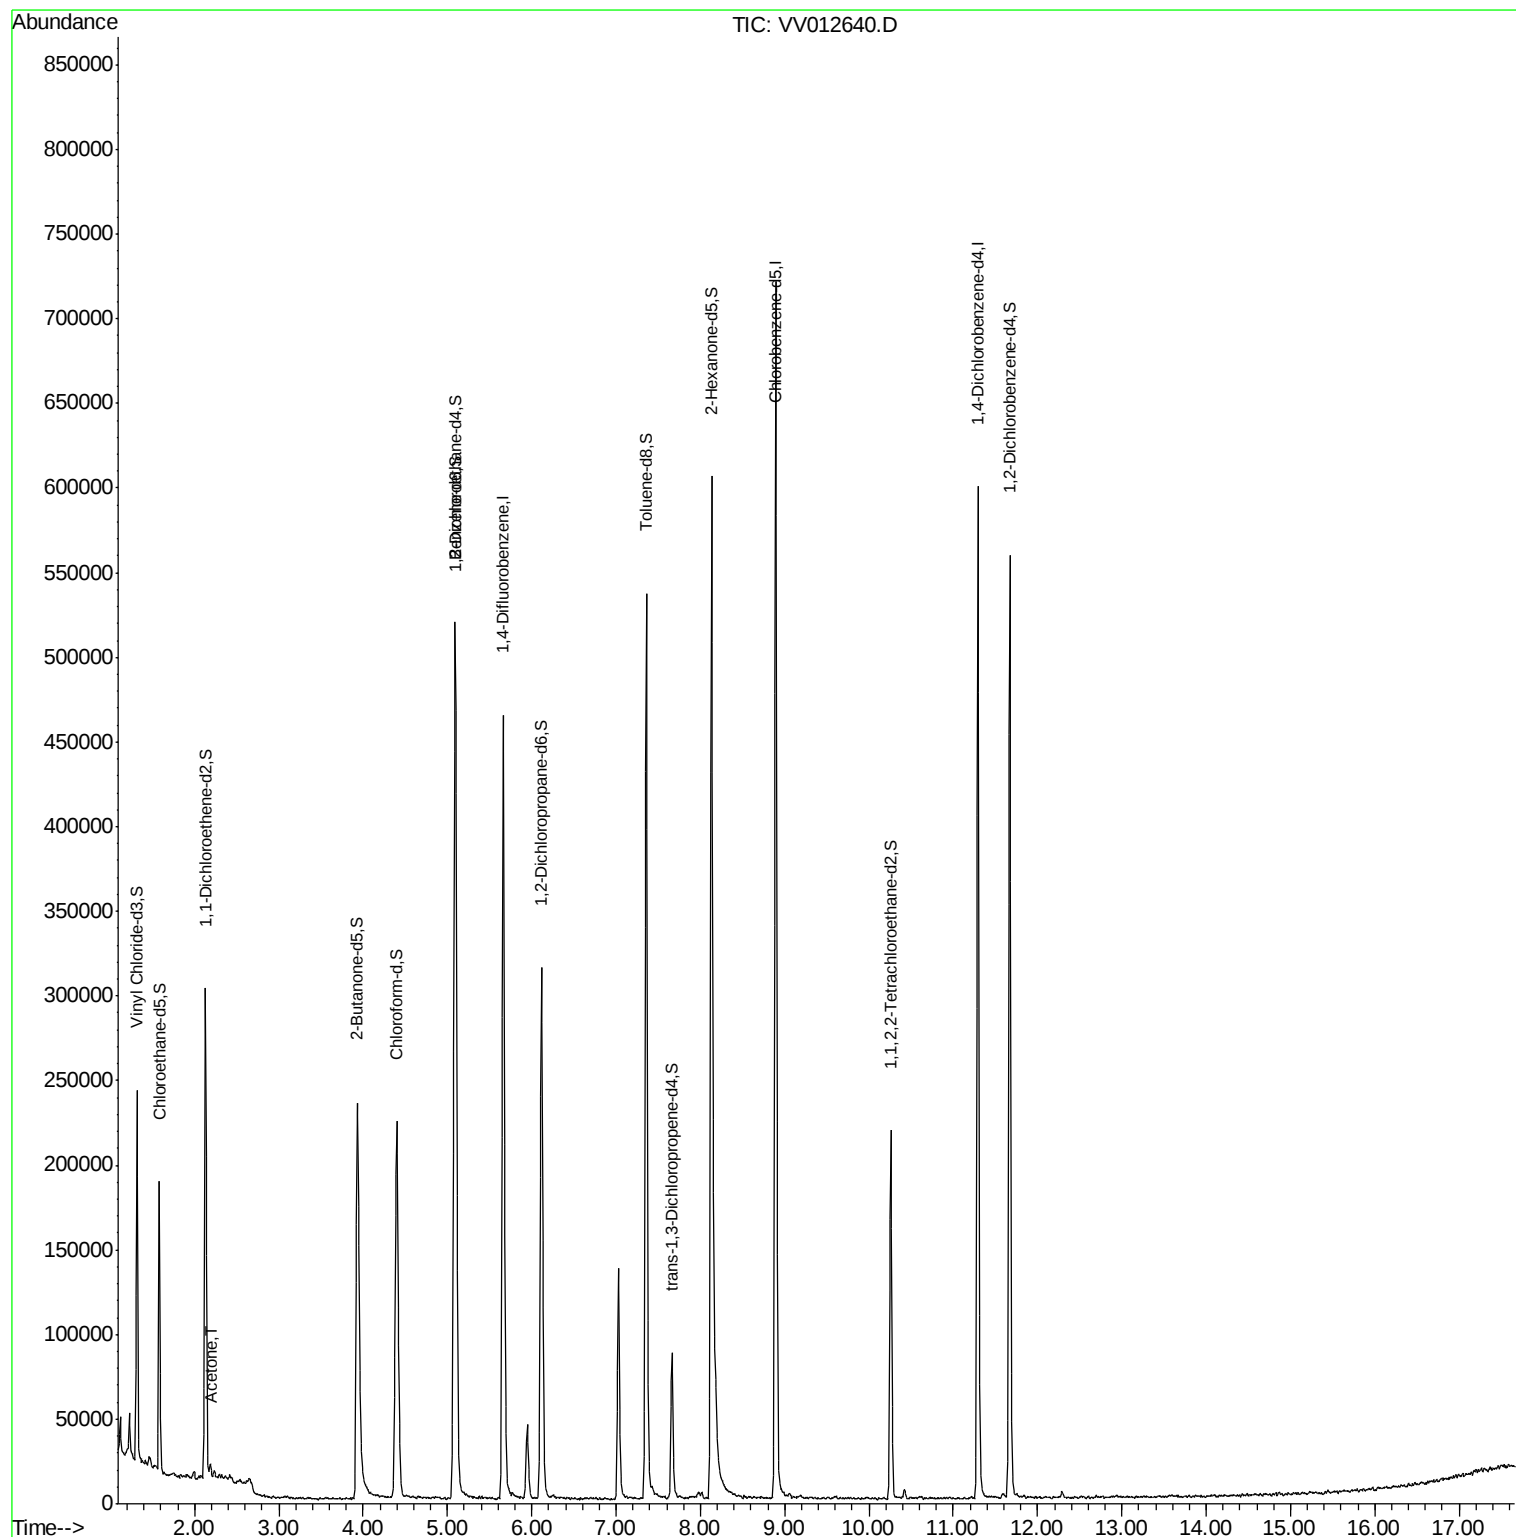

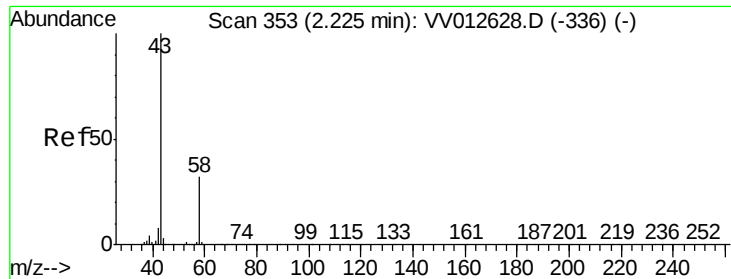

#13

Acetone

Concen: 1.809 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.04 min

Lab File: VV012640.D

Acq: 09 Sep 2019 23:08

Instrument :

MSVOA_V

ClientSampleId :

H0BM9

Tot Ion: 43 Resp: 6800

Ion Ratio Lower Upper

43 100

58 33.2 0.0 67.4

