


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090919\
 Data File : VV012621.D
 Acq On : 09 Sep 2019 13:07
 Operator : SY/MD
 Sample : BFB33
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB33

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Sep 12 07:16:59 2019

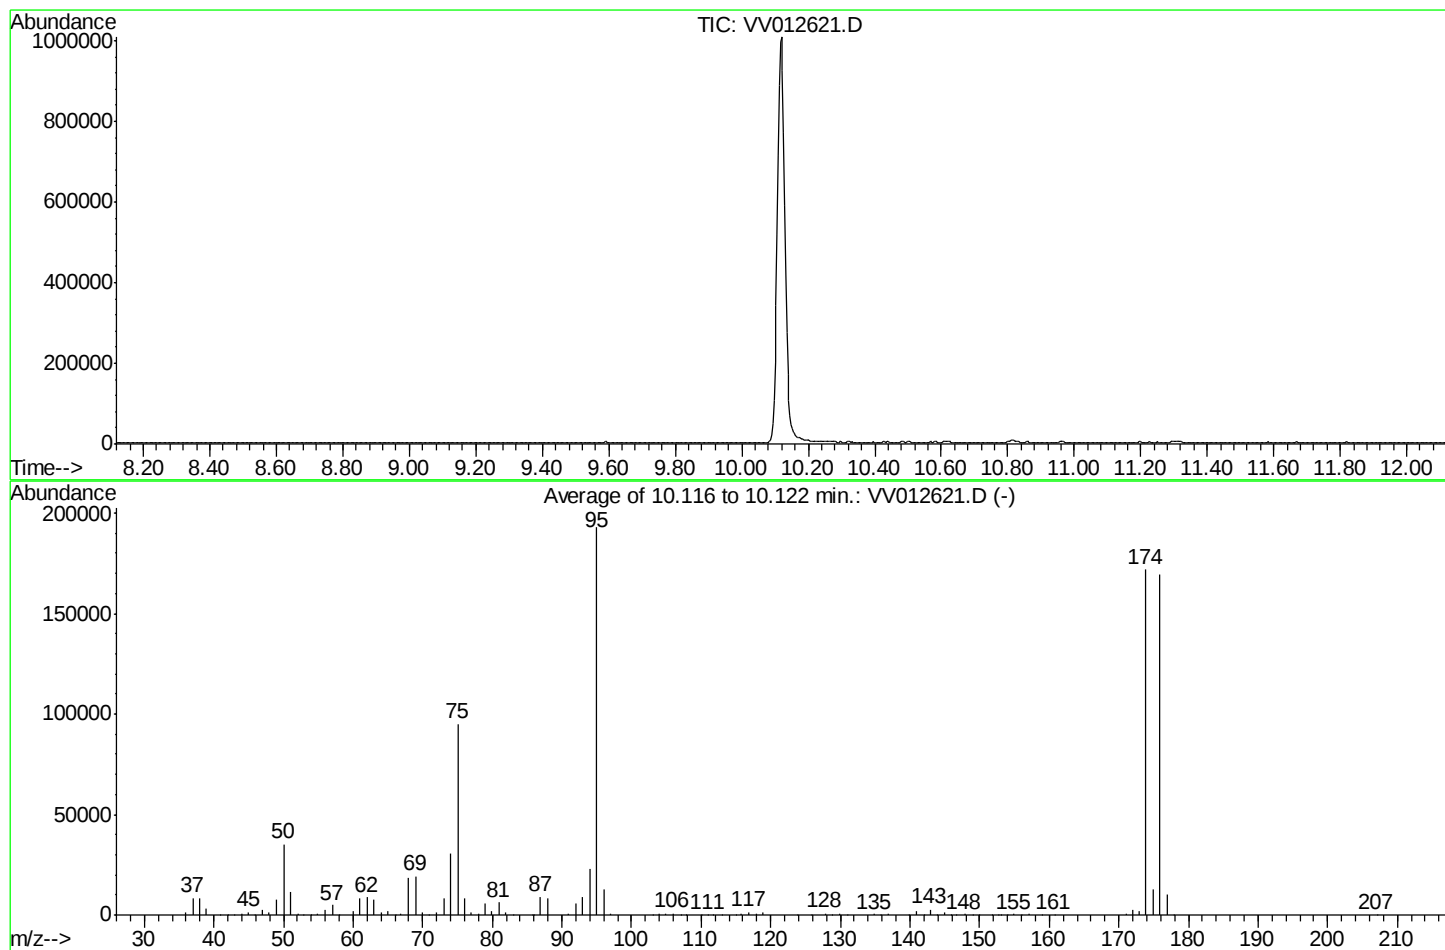

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	35277	PASS
75	95	30	80	49.2	94965	PASS
95	95	100	100	100.0	192917	PASS
96	95	5	9	6.5	12591	PASS
173	174	0.00	2	1.1	1972	PASS
174	95	50	120	89.1	171818	PASS
175	174	5	9	7.4	12764	PASS
176	174	95	101	98.5	169194	PASS
177	176	5	9	6.1	10307	PASS

m/z	Abundance
36.00	1866.0
37.00	9076.0
38.00	8635.0
39.00	3707.0
39.90	1577.0
40.90	166.0
41.90	104.0
43.00	188.0
44.00	2410.0
45.00	1527.0
45.80	327.0
47.00	2962.0
47.90	1108.0
49.00	7608.0
50.00	36184.0
51.00	11215.0
52.00	631.0
52.90	198.0
54.00	128.0
54.90	537.0
56.00	2888.0
57.00	5205.0
57.90	155.0
60.00	1816.0
61.00	8597.0
62.00	9171.0
63.00	7916.0
64.00	1279.0
65.00	2229.0
66.00	319.0
66.90	438.0
68.00	19592.0
69.00	20568.0
70.00	1294.0
70.80	110.0
72.00	1075.0
73.00	8608.0
74.00	32312.0
75.00	97784.0
76.00	8520.0
77.00	1035.0
78.00	727.0
78.90	5810.0
79.90	1916.0
80.90	6367.0
81.90	1391.0
82.90	154.0
85.70	312.0
86.90	9745.0
87.90	8571.0
90.90	803.0
92.00	6035.0
93.00	8862.0
94.00	23304.0
95.00	197696.0
96.00	13221.0
97.00	409.0
103.00	110.0
103.90	683.0
104.80	352.0
106.00	773.0
107.00	128.0
109.90	169.0
111.00	128.0
111.60	155.0
112.90	176.0
114.90	195.0
115.80	737.0
116.90	1324.0
117.90	721.0
118.90	1234.0
123.80	111.0
127.90	742.0
128.80	345.0
129.80	684.0
130.90	452.0
134.90	417.0
135.70	119.0
136.80	392.0
139.90	160.0
140.90	1799.0
141.90	271.0
142.90	2687.0
143.80	178.0
144.90	979.0
145.90	351.0
147.80	544.0
149.00	150.0
149.90	221.0
151.80	106.0
152.60	174.0
153.10	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

154.10	186.0
154.90	552.0
156.00	132.0
157.10	414.0
159.00	315.0
160.70	273.0
171.00	407.0
172.00	2889.0
173.00	2008.0
173.90	171520.0
174.90	12883.0
175.90	170176.0
176.90	10611.0
178.00	295.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	1811.0
37.00	9000.0
38.00	8697.0
39.00	3320.0
39.90	1411.0
40.90	149.0
43.00	240.0
44.00	2346.0
44.90	1642.0
45.90	327.0
46.90	2963.0
47.90	1105.0
49.00	7827.0
50.00	36488.0
51.00	11619.0
52.10	586.0
52.90	183.0
53.90	121.0
54.90	556.0
56.00	2827.0
57.00	5085.0
60.00	1863.0
61.00	8775.0
62.00	9052.0
63.00	7784.0
64.00	1266.0
65.00	2242.0
66.00	242.0
66.90	519.0
68.00	19040.0
69.00	20096.0
70.00	1227.0
70.90	112.0
72.00	1128.0
73.00	8899.0
74.00	31984.0
75.00	98560.0
76.10	8542.0
77.00	964.0
78.00	841.0
78.90	5816.0
79.90	1955.0
80.90	6411.0
81.90	1352.0
83.00	153.0
85.70	358.0
86.00	274.0
86.90	9567.0
87.90	8418.0
90.90	693.0
92.00	5860.0
93.00	9254.0
94.00	23552.0
95.00	198912.0
96.00	13000.0
97.00	359.0
103.90	668.0
104.80	370.0
106.00	839.0
107.80	115.0
109.90	209.0
111.00	136.0
111.60	147.0
112.90	196.0
115.00	197.0
115.80	703.0
116.90	1301.0
117.90	696.0
118.90	1026.0
123.80	158.0
125.80	107.0
127.90	770.0
128.90	325.0
129.80	750.0
130.90	390.0
134.90	422.0
135.70	137.0
136.80	361.0
139.90	102.0
140.90	1809.0
141.90	292.0
142.90	2788.0
143.80	194.0
144.90	1045.0
145.90	351.0
147.90	606.0
149.00	149.0
149.90	241.0
151.80	145.0
152.60	160.0
154.10	184.0
154.90	597.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

156.00	135.0
157.10	471.0
158.90	322.0
160.70	278.0
171.00	427.0
171.90	2868.0
173.00	2055.0
173.90	177344.0
174.90	13171.0
175.90	175104.0
176.90	10678.0
177.90	306.0
207.10	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	1565.0
37.00	7953.0
38.00	7818.0
39.00	2912.0
39.90	1251.0
40.90	141.0
43.00	236.0
44.00	2287.0
44.90	1537.0
45.90	311.0
46.90	2660.0
47.90	975.0
49.00	7263.0
50.00	33160.0
51.00	10762.0
52.10	492.0
52.90	203.0
53.90	138.0
55.00	512.0
56.00	2502.0
57.00	4472.0
60.00	1823.0
61.00	8211.0
62.00	8350.0
63.00	6779.0
64.00	1240.0
65.00	1982.0
66.00	187.0
66.90	552.0
68.00	16880.0
69.00	17656.0
70.00	1110.0
71.00	138.0
71.90	1025.0
73.00	8327.0
74.00	28720.0
75.00	88552.0
76.10	7855.0
77.00	1053.0
78.00	802.0
78.90	5327.0
79.90	1785.0
80.90	5807.0
81.90	1236.0
83.00	119.0
85.80	311.0
86.00	266.0
86.90	8465.0
87.90	7508.0
90.90	601.0
92.00	5368.0
93.00	8504.0
94.00	21936.0
95.00	182144.0
96.00	11554.0
97.00	309.0
103.90	681.0
104.90	346.0
105.90	840.0
107.90	146.0
110.00	204.0
111.00	166.0
112.90	178.0
115.00	180.0
115.80	616.0
116.90	1240.0
117.90	639.0
118.90	871.0
123.80	164.0
127.80	699.0
128.90	308.0
129.90	712.0
130.90	295.0
134.90	353.0
135.70	122.0
136.80	320.0
140.90	1645.0
142.00	241.0
142.90	2584.0
143.90	177.0
144.90	959.0
145.90	293.0
146.60	101.0
147.90	561.0
149.10	134.0
150.00	198.0
151.80	150.0
152.60	109.0
154.00	171.0
154.90	546.0
155.90	118.0
157.10	405.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

158.90	266.0
160.80	286.0
171.00	334.0
171.90	2738.0
173.00	1855.0
173.90	166592.0
175.00	12239.0
175.90	162304.0
176.90	9634.0
177.80	378.0
207.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.10	148.0
37.20	133.0
38.90	161.0
39.90	1466.0
43.90	1408.0
45.10	102.0
48.80	117.0
51.80	120.0
73.90	101.0
131.00	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33