

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV031991.D
 Acq On : 09 Sep 2023 11:21
 Operator : SY/MD
 Sample : VV0909WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK359

Quant Time: Sep 09 21:53:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 09 21:51:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	127500	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	125800	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	68936	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	23891	5.548	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	111.000%	
7) Chloroethane-d5	1.532	69	28896	5.858	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	117.200%	
11) 1,1-Dichloroethene-d2	2.060	65	14142	5.580	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	111.600%	
20) 2-Butanone-d5	3.802	46	112278	53.862	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.720%	
24) Chloroform-d	4.256	84	69462	4.766	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
26) 1,2-Dichloroethane-d4	4.950	65	36546	4.866	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.400%	
32) Benzene-d6	4.963	84	141414	4.940	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
36) 1,2-Dichloropropane-d6	5.992	67	49025	4.857	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.200%	
41) Toluene-d8	7.249	98	125420	4.722	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
43) trans-1,3-Dichloroprop...	7.561	79	13655	3.710	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.200%	
46) 2-Hexanone-d5	8.030	63	90826	46.280	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.560%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	34263	4.731	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152	46211	4.139	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	82.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.449	84	2448	0.262	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031991.D
Acq On : 09 Sep 2023 11:21
Operator : SY/MD
Sample : VV0909WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK359

Quant Time: Sep 09 21:53:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 09 21:51:31 2023
Response via : Initial Calibration

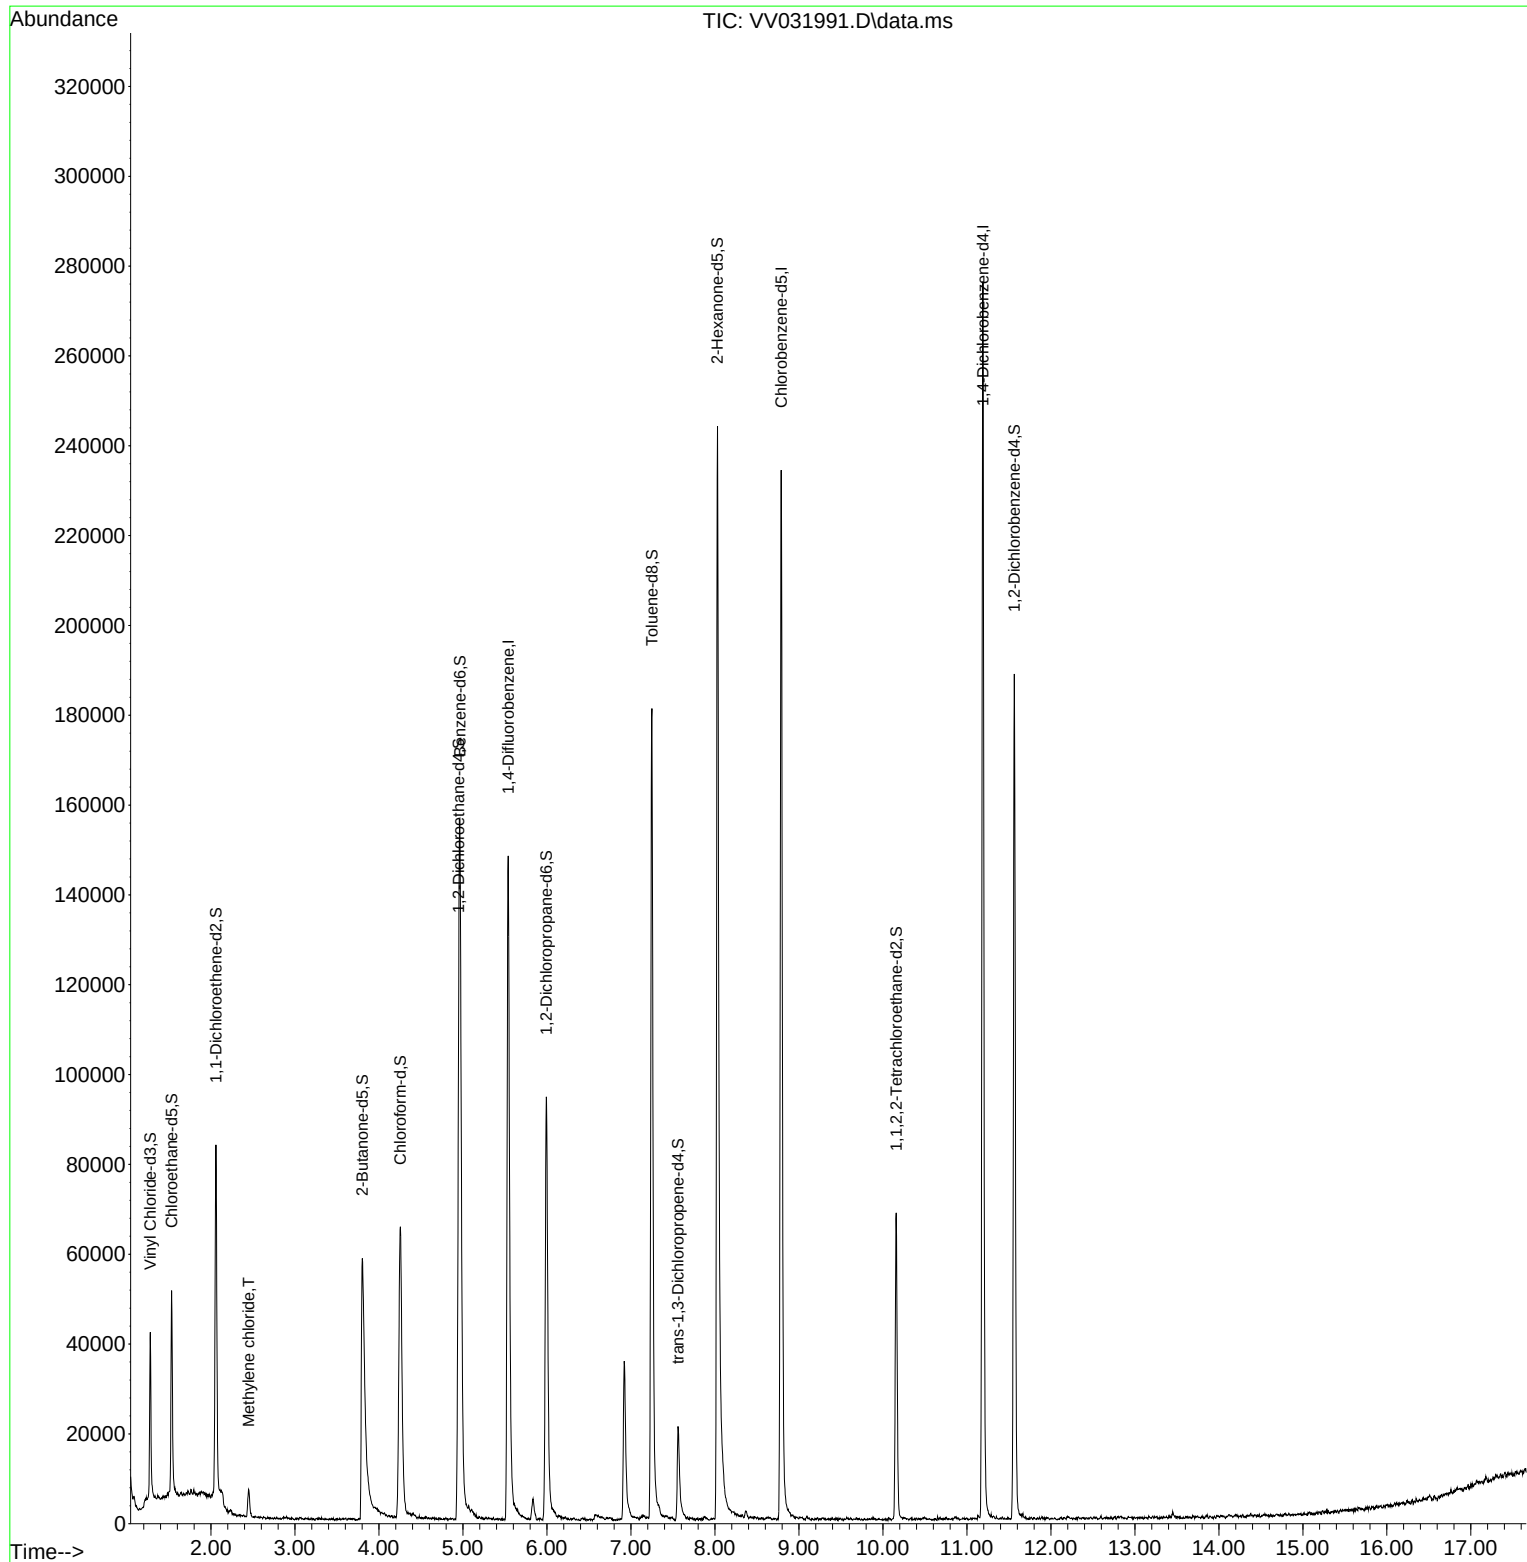

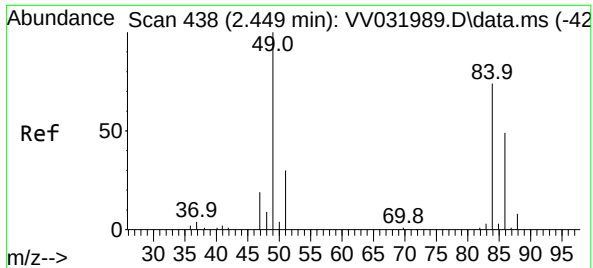

#16
Methylene chloride
Concen: 0.262 ug/L
RT: 2.449 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV031991.D
Acq: 09 Sep 2023 11:21

Instrument :
MSVOA_V
ClientSampleId :
VBLK359

Tgt Ion:	84	Resp:	2448
Ion	Ratio	Lower	Upper
84	100		
86	55.4	42.6	79.2
49	109.8	88.5	164.4

