

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV032008.D
 Acq On : 09 Sep 2023 18:19
 Operator : SY/MD
 Sample : 04307-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4N7

Quant Time: Sep 09 21:57:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 09 21:51:31 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 09/15/2023
 Supervised By :Semsettin Yesilyurt 09/15/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	125765	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	124188	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	65421	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	21099	4.967	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	99.400%	
7) Chloroethane-d5	1.532	69	26799	5.507	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	110.200%	
11) 1,1-Dichloroethene-d2	2.060	65	12353	4.941	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	98.800%	
20) 2-Butanone-d5	3.806	46	108131	52.588	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.180%	
24) Chloroform-d	4.256	84	62773	4.367	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.400%	
26) 1,2-Dichloroethane-d4	4.950	65	34017	4.592	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.800%	
32) Benzene-d6	4.966	84	130678	4.624	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
36) 1,2-Dichloropropane-d6	5.995	67	45371	4.553	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.000%	
41) Toluene-d8	7.249	98	112400	4.286	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	7.564	79	12093	3.328	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	66.600%	
46) 2-Hexanone-d5	8.030	63	79759	41.168	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	82.340%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	30579	4.277	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	85.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152	41633	3.930	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	78.600%#	
Target Compounds					Qvalue	
13) Acetone	2.130	43	50612	41.774	ug/L	73
15) Methyl Acetate	2.384	43	18321	7.420	ug/L	100
16) Methylene chloride	2.452	84	3166	0.344	ug/L	98
21) 2-Butanone	3.915	43	10594m	6.173	ug/L	
40) 4-Methyl-2-pentanone	7.178	43	7880	1.595	ug/L #	90
42) Toluene	7.330	91	4169	0.131	ug/L	98
55) Styrene	9.519	104	2151	0.094	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032008.D
Acq On : 09 Sep 2023 18:19
Operator : SY/MD
Sample : 04307-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH4N7

Quant Time: Sep 09 21:57:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 09 21:51:31 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 09/15/2023
Supervised By :Semsettin Yesilyurt 09/15/2023

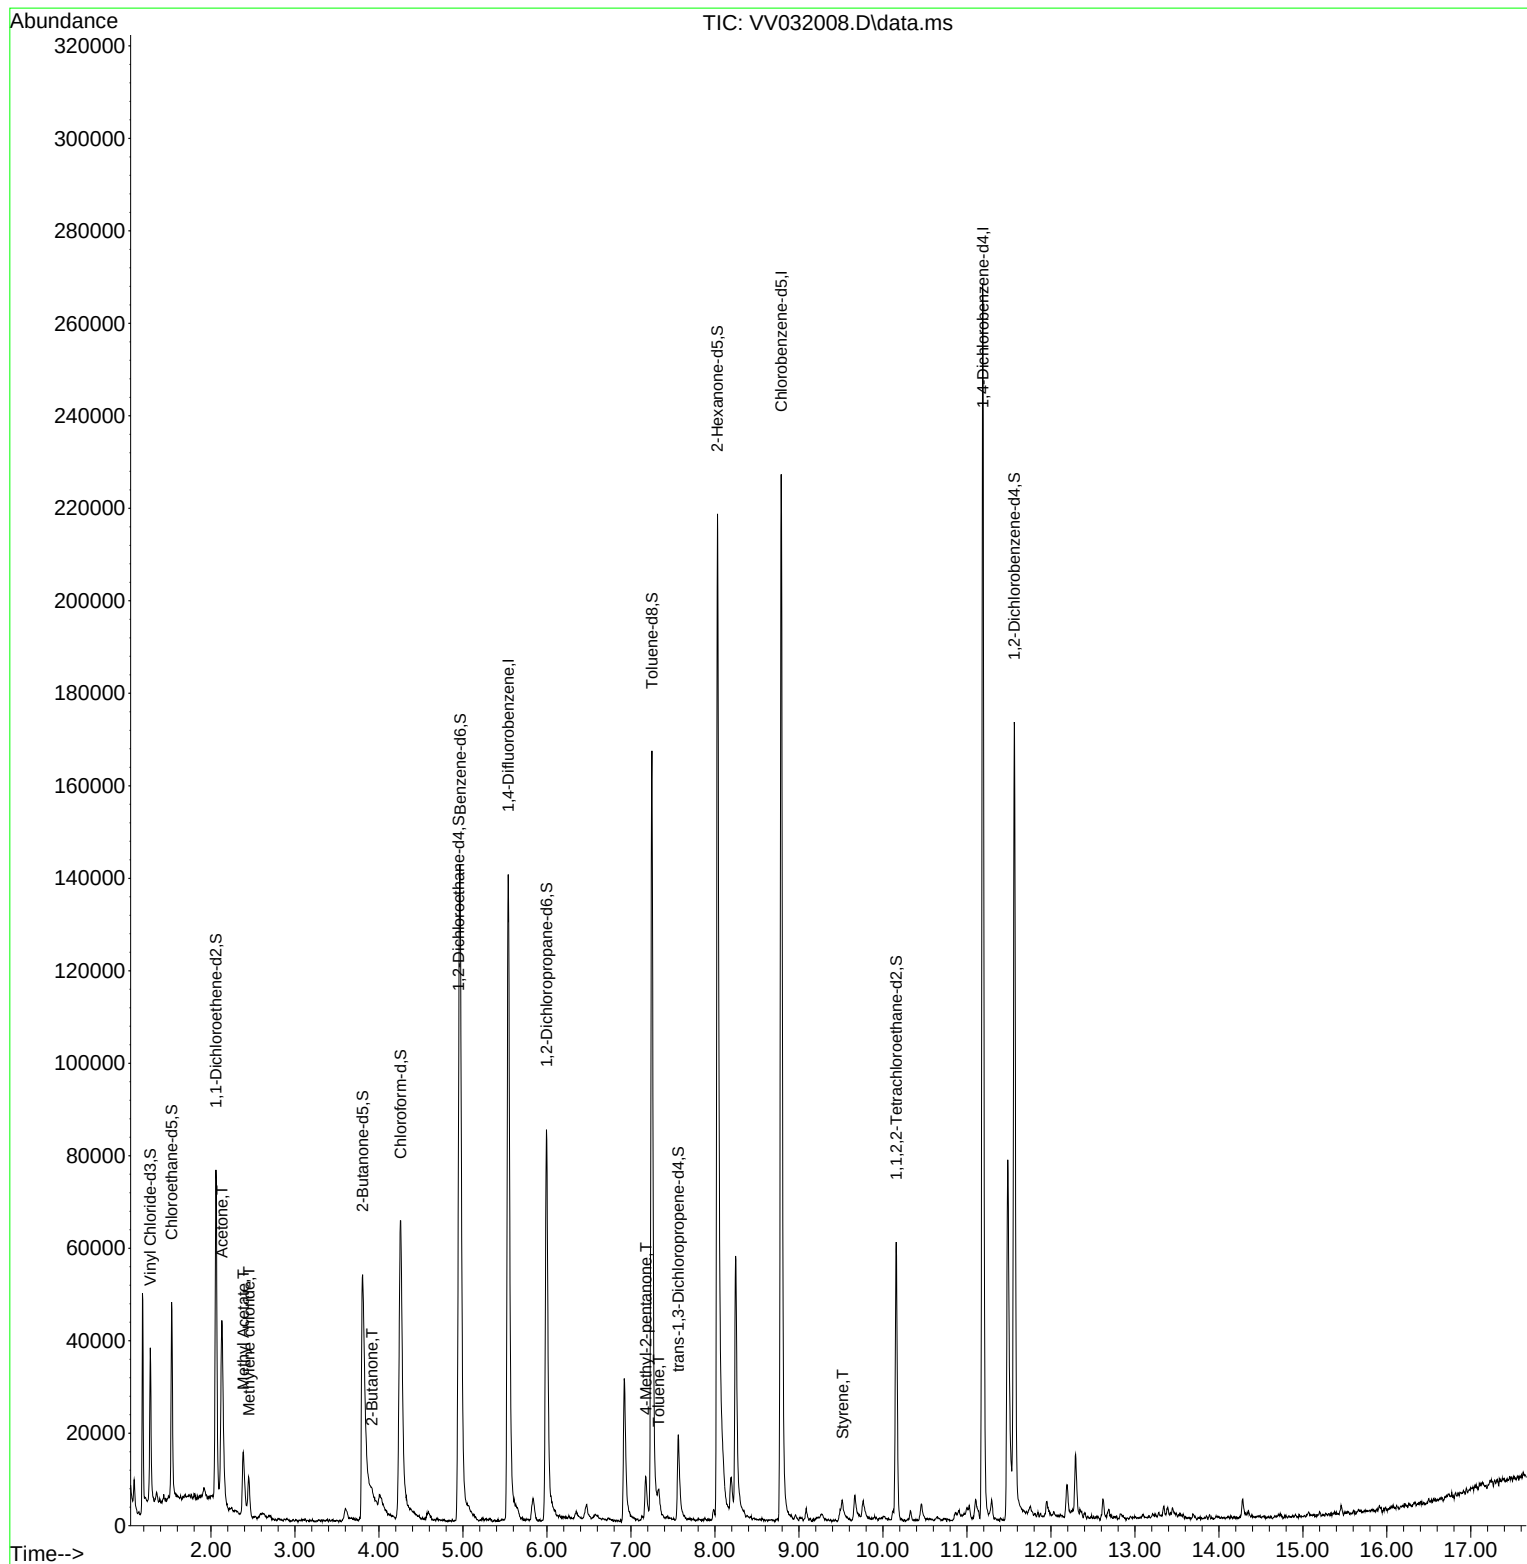

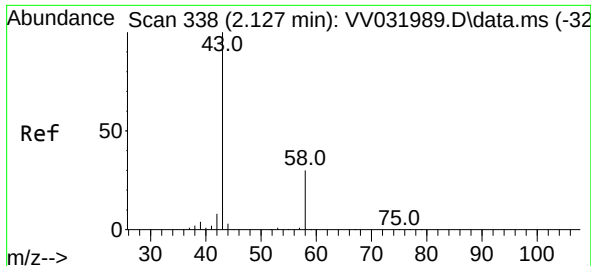

#13

Acetone

Concen: 41.774 ug/L

RT: 2.130 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV032008.D

Acq: 09 Sep 2023 18:19

Instrument :

MSVOA_V

ClientSampleId :

BH4N7

Tgt Ion: 43 Resp: 5061

Ion Ratio Lower Upper

43 100





58 30.5 0.0 37.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 09/15/2023

Supervised By :Semsettin Yesilyurt 09/15/2023

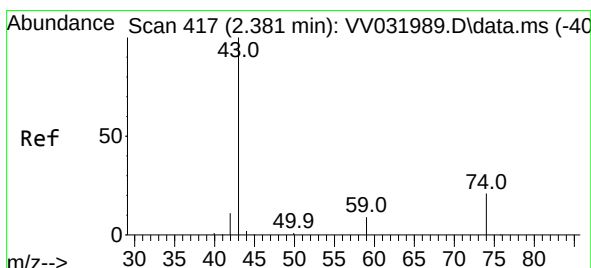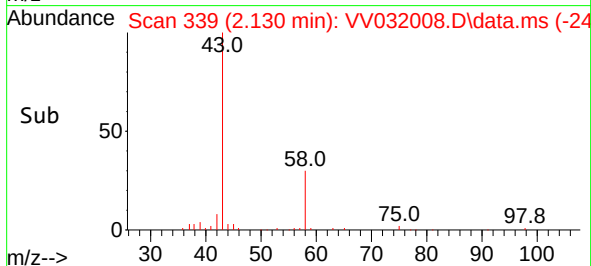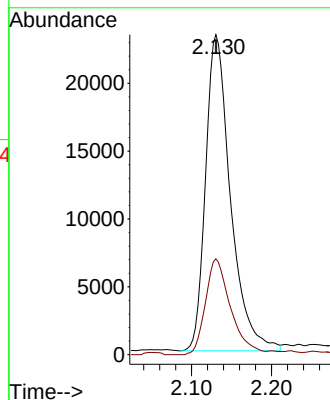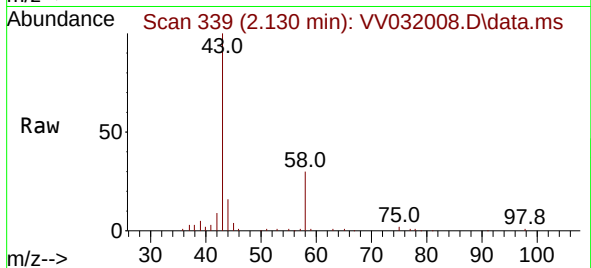

#15

Methyl Acetate

Concen: 7.420 ug/L

RT: 2.384 min Scan# 418

Delta R.T. 0.003 min

Lab File: VV032008.D




Acq: 09 Sep 2023 18:19


Tgt Ion: 43 Resp: 18321

Ion Ratio Lower Upper

43 100


74 23.0 18.3 27.5

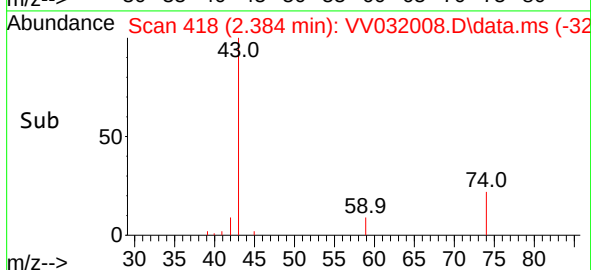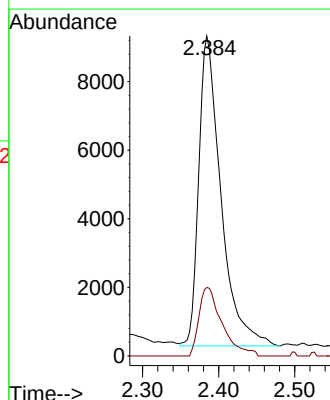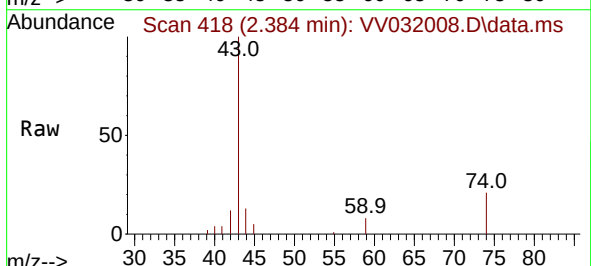

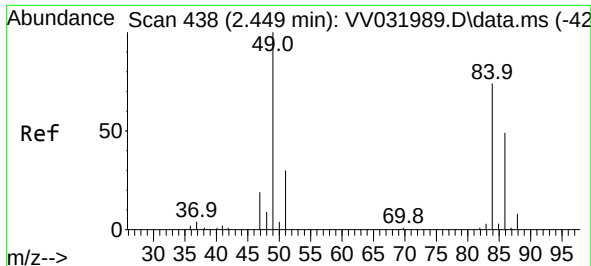

#16
Methylene chloride
Concen: 0.344 ug/L
RT: 2.452 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV032008.D
Acq: 09 Sep 2023 18:19




Instrument :
MSVOA_V
ClientSampleId :
BH4N7

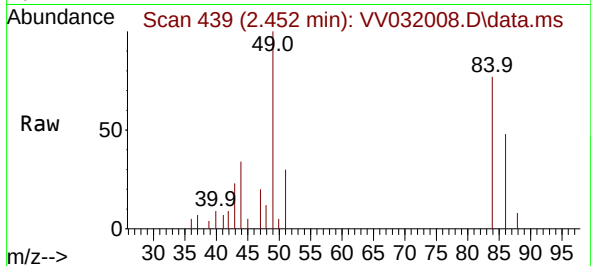

Tgt Ion: 84 Resp: 3160
Ion Ratio Lower Upper
84 100
86 62.3 42.6 79.2
49 129.7 88.5 164.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 09/15/2023
Supervised By :Semsettin Yesilyurt 09/15/2023

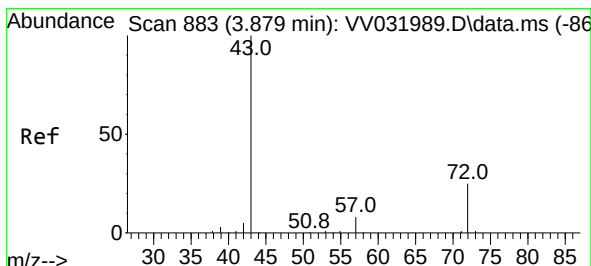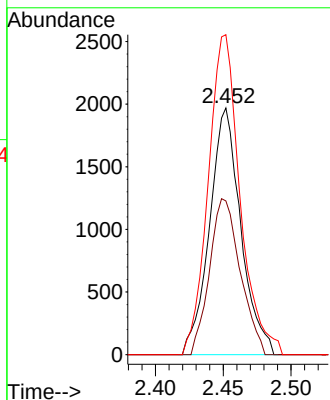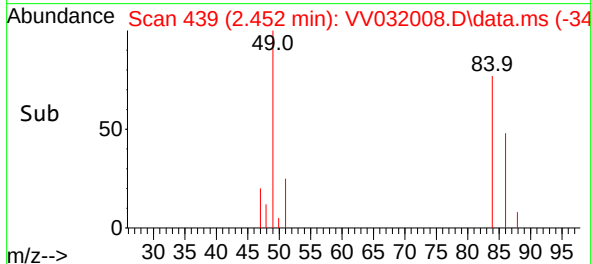

#21
2-Butanone
Concen: 6.173 ug/L m
RT: 3.915 min Scan# 894
Delta R.T. 0.036 min
Lab File: VV032008.D
Acq: 09 Sep 2023 18:19

Tgt Ion: 43 Resp: 10594
Ion Ratio Lower Upper
43 100
72 0.4 9.0 27.0#

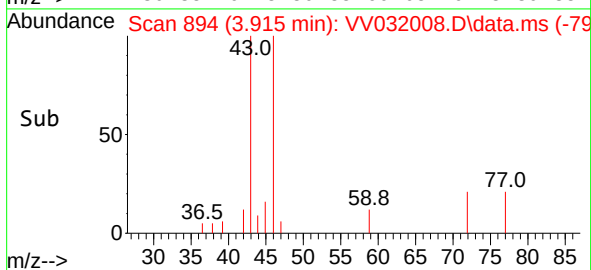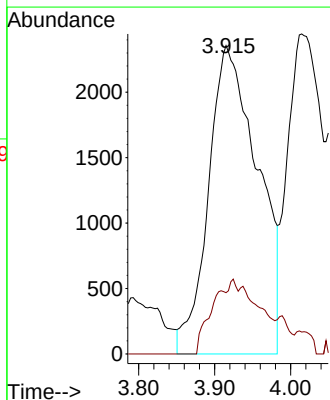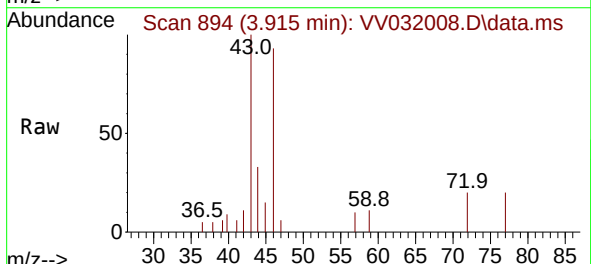

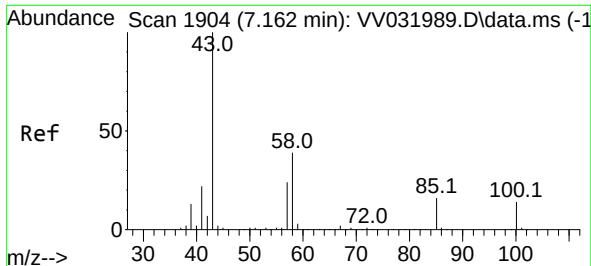

#40

4-Methyl-2-pentanone

Concen: 1.595 ug/L

RT: 7.178 min Scan# 1909

Delta R.T. 0.016 min

Lab File: VV032008.D

Acq: 09 Sep 2023 18:19

Instrument :

MSVOA_V

ClientSampleId :





BH4N7

Tgt Ion: 43 Resp: 7880
 Ion Ratio Lower Upper
 43 100
 58 35.3 29.0 43.6
 100 0.0 10.7 16.1

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 09/15/2023
 Supervised By :Semsettin Yesilyurt 09/15/2023

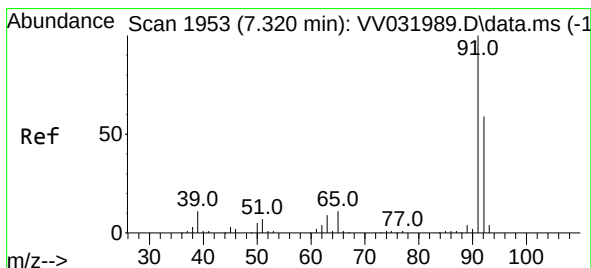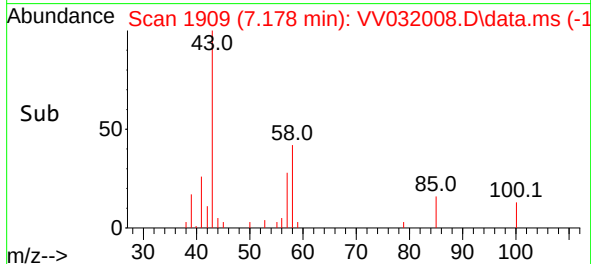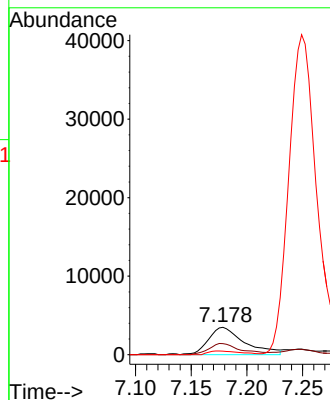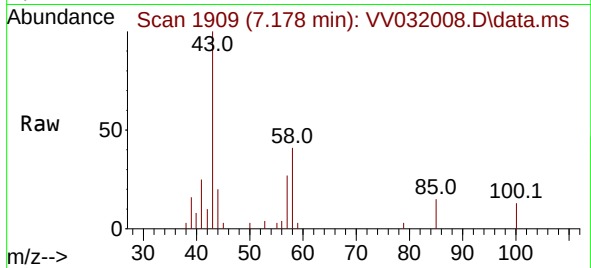

#42

Toluene

Concen: 0.131 ug/L




RT: 7.330 min Scan# 1956


Delta R.T. 0.010 min

Lab File: VV032008.D

Acq: 09 Sep 2023 18:19

Tgt Ion: 91 Resp: 4169
 Ion Ratio Lower Upper
 91 100
 92 59.2 40.5 75.1

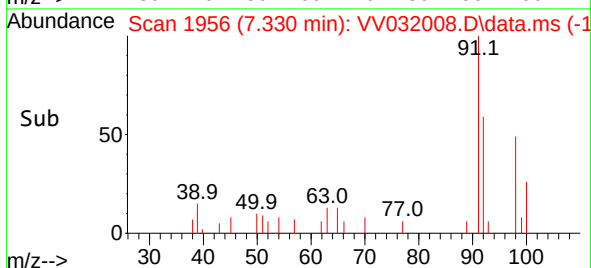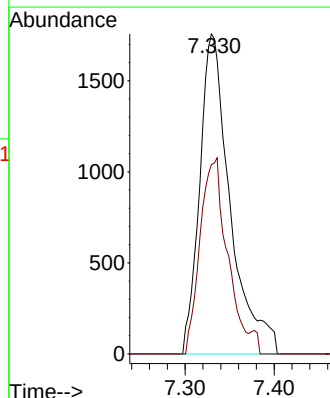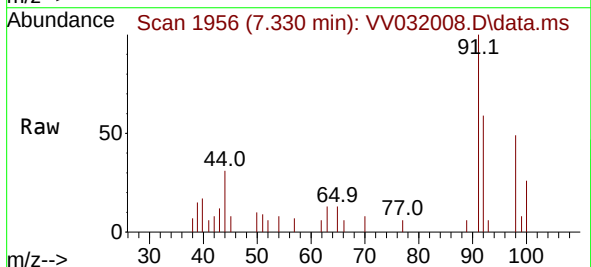

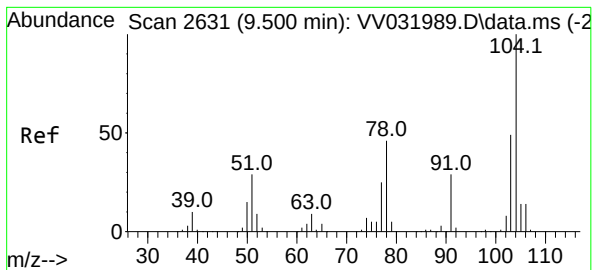

#55
 Styrene
 Concen: 0.094 ug/L
 RT: 9.519 min Scan# 20
 Delta R.T. 0.019 min
 Lab File: VV032008.D
 Acq: 09 Sep 2023 18:19

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4N7

Tgt Ion:104 Resp: 215
 Ion Ratio Lower Upper
 104 100
 78 49.0 32.1 59.7

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 09/15/2023
 Supervised By :Semsettin Yesilyurt 09/15/2023

