

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV031990.D
 Acq On : 09 Sep 2023 10:21
 Operator : SY/MD
 Sample : VV0909WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK358

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	33980	40499	9.10%	1.180%
2	1.532	146	153	164	rVB	40414	46767	10.51%	1.363%
3	2.059	308	317	329	rBV	68924	100038	22.49%	2.915%
4	2.449	429	438	450	rBV2	6076	10903	2.45%	0.318%
5	3.805	851	860	888	rBV2	49340	153472	34.50%	4.471%
6	4.256	981	1000	1024	rBV	55143	147872	33.24%	4.308%
7	4.963	1204	1220	1248	rBV2	136359	354074	79.60%	10.316%
8	5.538	1385	1399	1422	rBV	147704	311970	70.13%	9.089%
9	5.834	1481	1491	1506	rVB7	3734	7684	1.73%	0.224%
10	5.995	1525	1541	1569	rBV	82477	182164	40.95%	5.307%
11	6.921	1818	1829	1854	rBV	31693	66909	15.04%	1.949%
12	7.249	1919	1931	1958	rBV	160872	295447	66.42%	8.608%
13	7.564	2017	2029	2046	rBV2	18564	38531	8.66%	1.123%
14	8.030	2164	2174	2216	rBV	215937	431128	96.92%	12.560%
15	8.789	2398	2410	2430	rBV	236464	401862	90.34%	11.708%
16	10.159	2822	2836	2847	rBV	60067	96654	21.73%	2.816%
17	11.188	3145	3156	3179	rBV	280231	444839	100.00%	12.960%
18	11.564	3261	3273	3295	rBV	164590	269399	60.56%	7.849%
19	13.207	3777	3784	3797	rBV7	4513	7019	1.58%	0.204%
20	13.448	3850	3859	3873	rBV2	10761	17661	3.97%	0.515%
21	13.686	3926	3933	3941	rBV5	5479	7528	1.69%	0.219%




Sum of corrected areas: 3432420

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031990.D
Acq On : 09 Sep 2023 10:21
Operator : SY/MD
Sample : VV0909WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

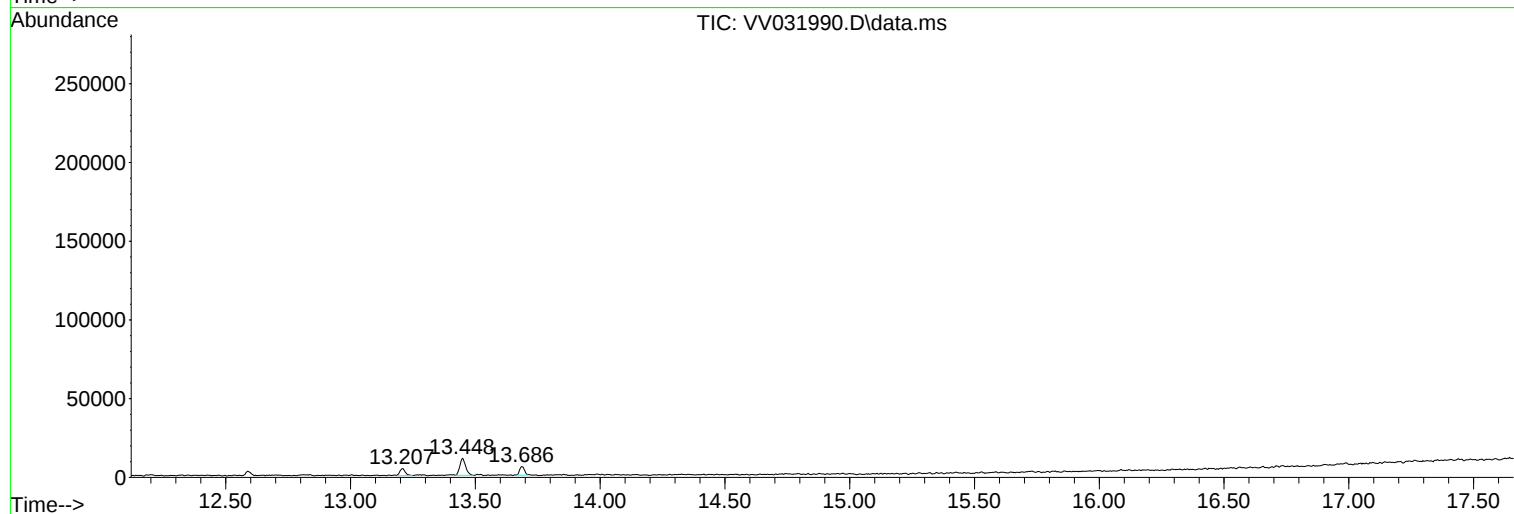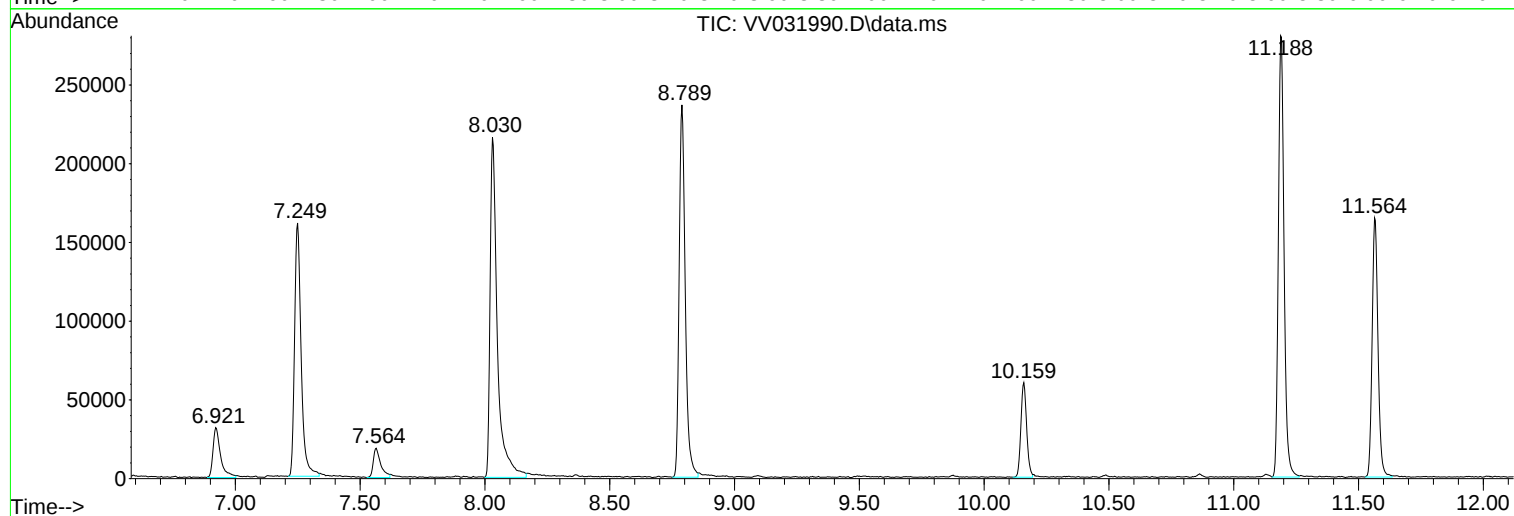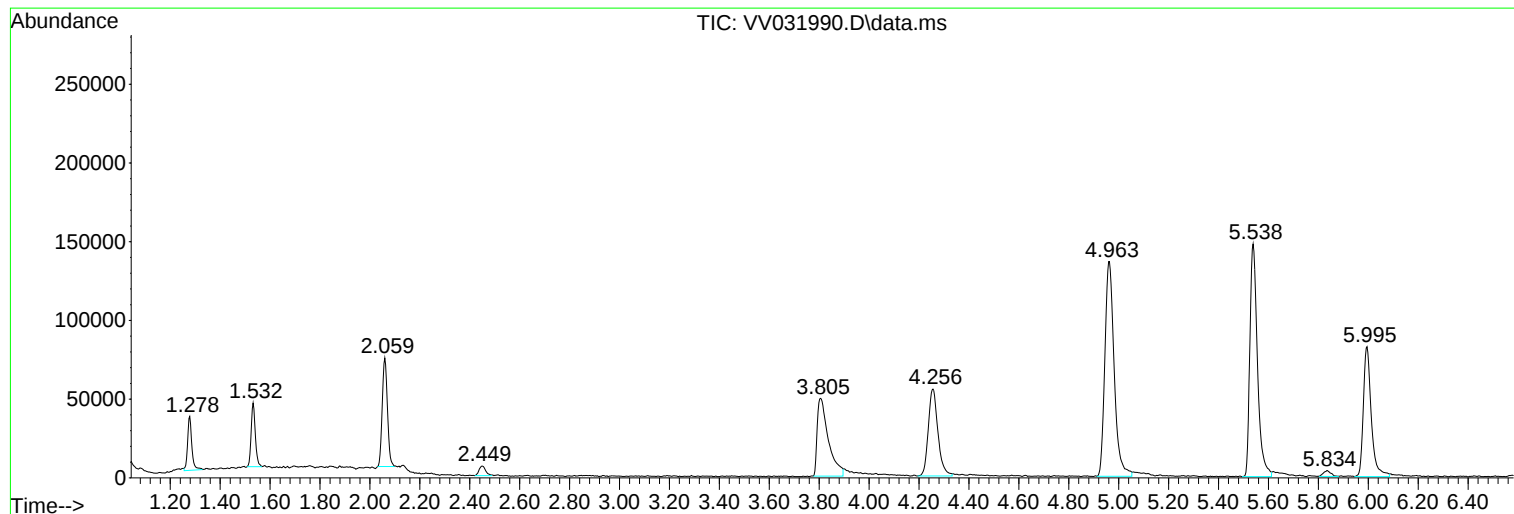

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031990.D
Acq On : 09 Sep 2023 10:21
Operator : SY/MD
Sample : VV0909WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031990.D
Acq On : 09 Sep 2023 10:21
Operator : SY/MD
Sample : VV0909WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK358

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc