

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV031994.D
 Acq On : 09 Sep 2023 12:37
 Operator : SY/MD
 Sample : VIBLK315
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK315

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	35671	38756	8.94%	1.107%
2	1.532	146	153	168	rVB	43064	51238	11.82%	1.464%
3	2.060	308	317	331	rBV	76281	110380	25.46%	3.154%
4	2.452	429	439	448	rBV3	3912	6247	1.44%	0.178%
5	3.809	849	861	897	rBV2	56392	190699	43.99%	5.449%
6	4.256	982	1000	1024	rBV	59372	158641	36.60%	4.533%
7	4.963	1203	1220	1247	rBV2	147821	381532	88.02%	10.902%
8	5.539	1389	1399	1423	rBV	148020	307165	70.86%	8.777%
9	5.834	1478	1491	1502	rBV9	3895	8346	1.93%	0.238%
10	5.995	1528	1541	1562	rBV	86542	188255	43.43%	5.379%
11	6.921	1817	1829	1849	rBV	32152	65322	15.07%	1.866%
12	7.249	1919	1931	1957	rBV	172444	319436	73.69%	9.127%
13	7.564	2020	2029	2049	rBV	18445	37796	8.72%	1.080%
14	8.030	2165	2174	2209	rBV	206650	417793	96.38%	11.938%
15	8.368	2271	2279	2291	rVB2	5994	9578	2.21%	0.274%
16	8.789	2397	2410	2436	rBV	232838	399452	92.15%	11.414%
17	10.159	2825	2836	2855	rBV	59629	96945	22.36%	2.770%
18	11.191	3145	3157	3182	rBV	272168	433475	100.00%	12.386%
19	11.564	3262	3273	3293	rBV	175708	278728	64.30%	7.964%




Sum of corrected areas: 3499784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031994.D
Acq On : 09 Sep 2023 12:37
Operator : SY/MD
Sample : VIBLK315
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

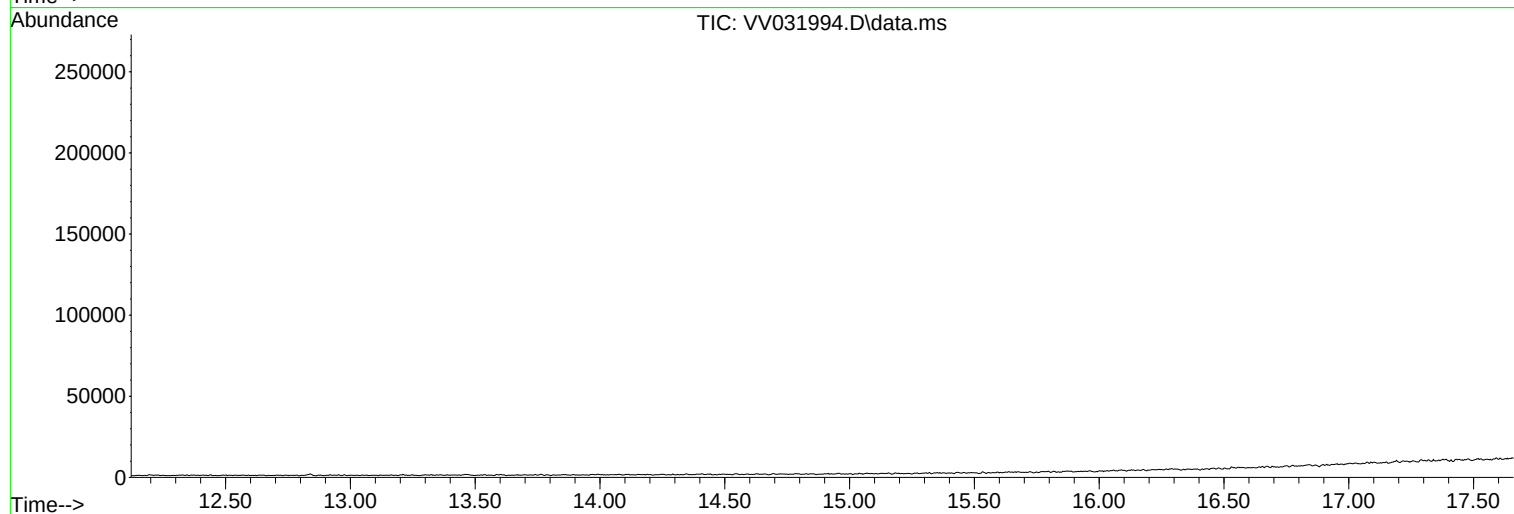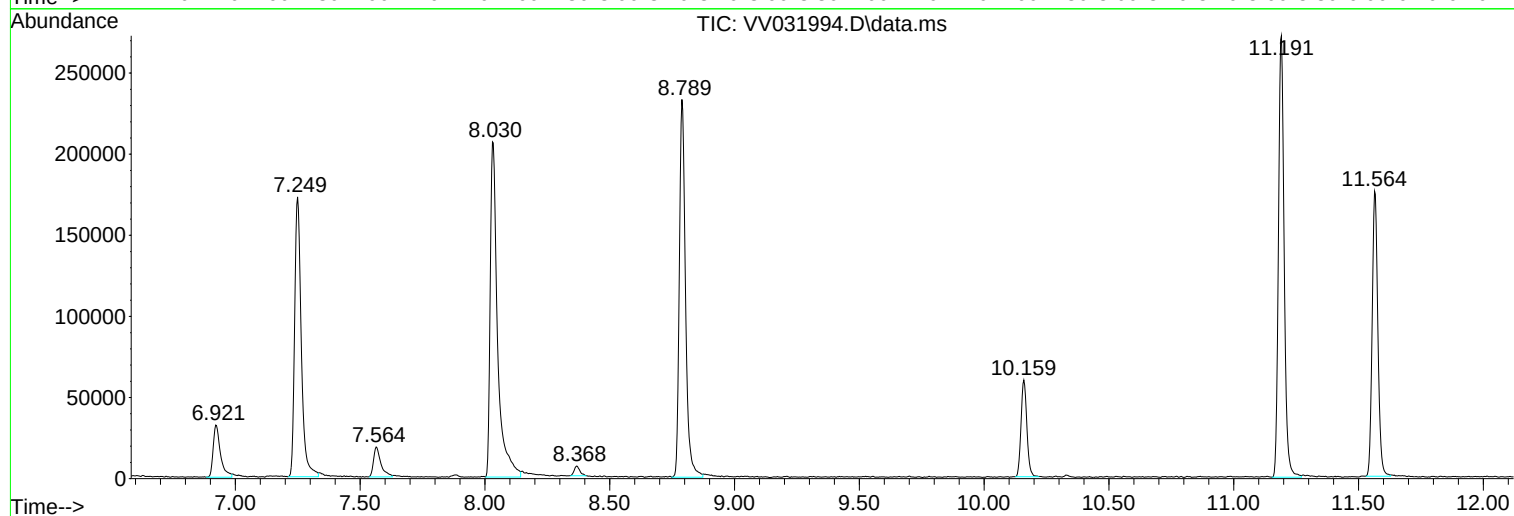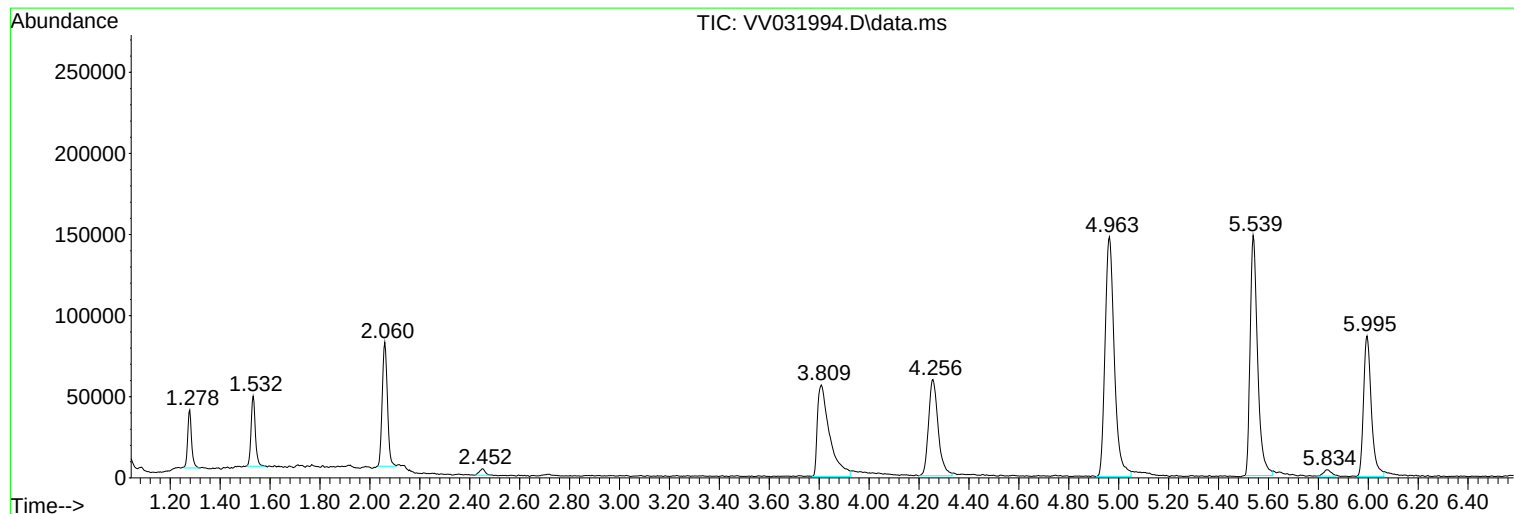

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031994.D
Acq On : 09 Sep 2023 12:37
Operator : SY/MD
Sample : VIBLK315
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031994.D
Acq On : 09 Sep 2023 12:37
Operator : SY/MD
Sample : VIBLK315
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc