

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV031996.D
 Acq On : 09 Sep 2023 13:26
 Operator : SY/MD
 Sample : 04267-11DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4D5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	88	rBV	31265	35640	6.68%	0.930%
2	1.532	146	153	171	rVB	38461	47195	8.85%	1.231%
3	2.059	308	317	331	rBV	65292	94153	17.65%	2.457%
4	2.449	427	438	449	rVB2	6125	10861	2.04%	0.283%
5	3.805	846	860	892	rBV2	60357	202113	37.88%	5.274%
6	4.256	980	1000	1029	rBV2	52970	144112	27.01%	3.760%
7	4.963	1202	1220	1249	rBV2	132012	338678	63.48%	8.837%
8	5.538	1386	1399	1428	rBV	184326	389363	72.98%	10.160%
9	5.837	1478	1492	1517	rBV	117968	250433	46.94%	6.535%
10	5.995	1528	1541	1566	rBV2	78616	164808	30.89%	4.300%
11	6.924	1819	1830	1854	rBV2	27958	59754	11.20%	1.559%
12	7.249	1919	1931	1954	rBV	151765	279281	52.35%	7.287%
13	7.564	2018	2029	2041	rBV2	16524	31782	5.96%	0.829%
14	8.030	2162	2174	2218	rBV	200174	406841	76.26%	10.616%
15	8.368	2269	2279	2288	rBV5	3424	6124	1.15%	0.160%
16	8.789	2398	2410	2438	rBV	293265	495314	92.84%	12.924%
17	10.159	2821	2836	2851	rBV	57281	92074	17.26%	2.403%
18	11.191	3145	3157	3176	rBV	332762	533512	100.00%	13.921%
19	11.567	3263	3274	3290	rBV	156885	250342	46.92%	6.532%




Sum of corrected areas: 3832380

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031996.D
Acq On : 09 Sep 2023 13:26
Operator : SY/MD
Sample : 04267-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

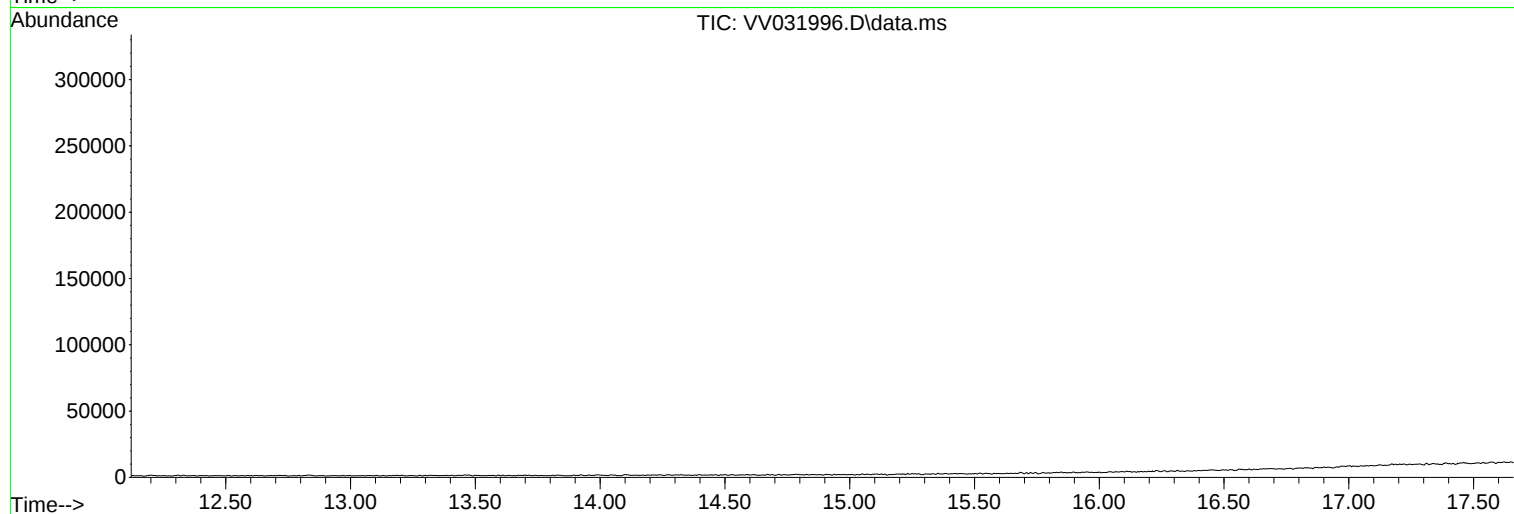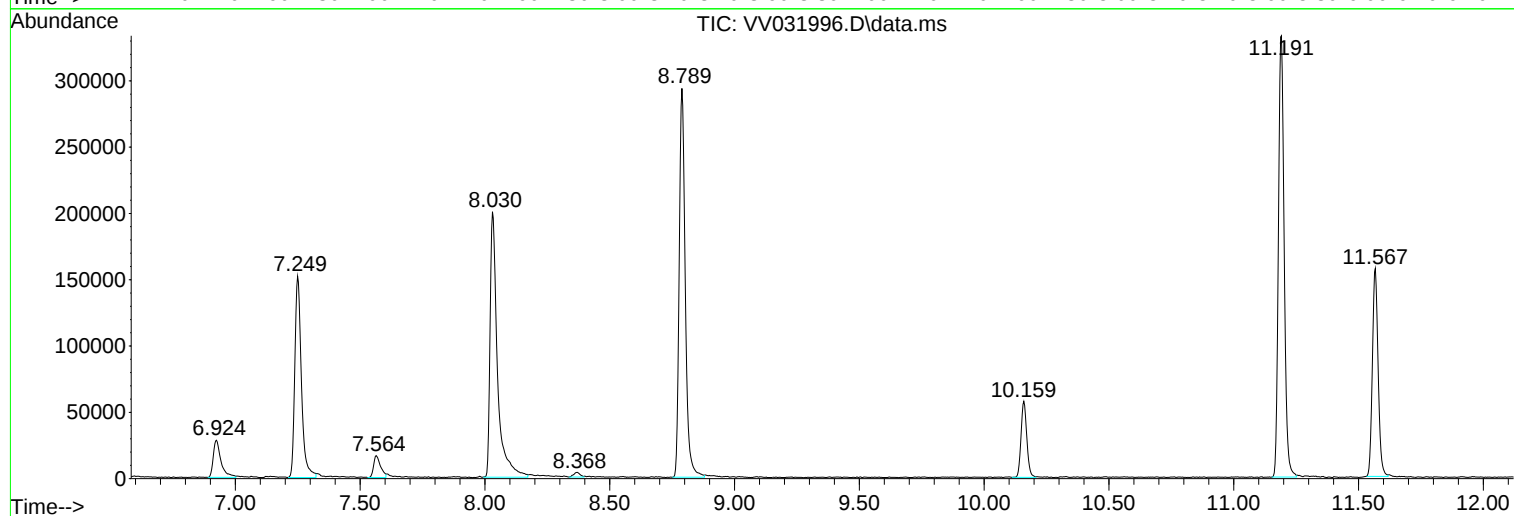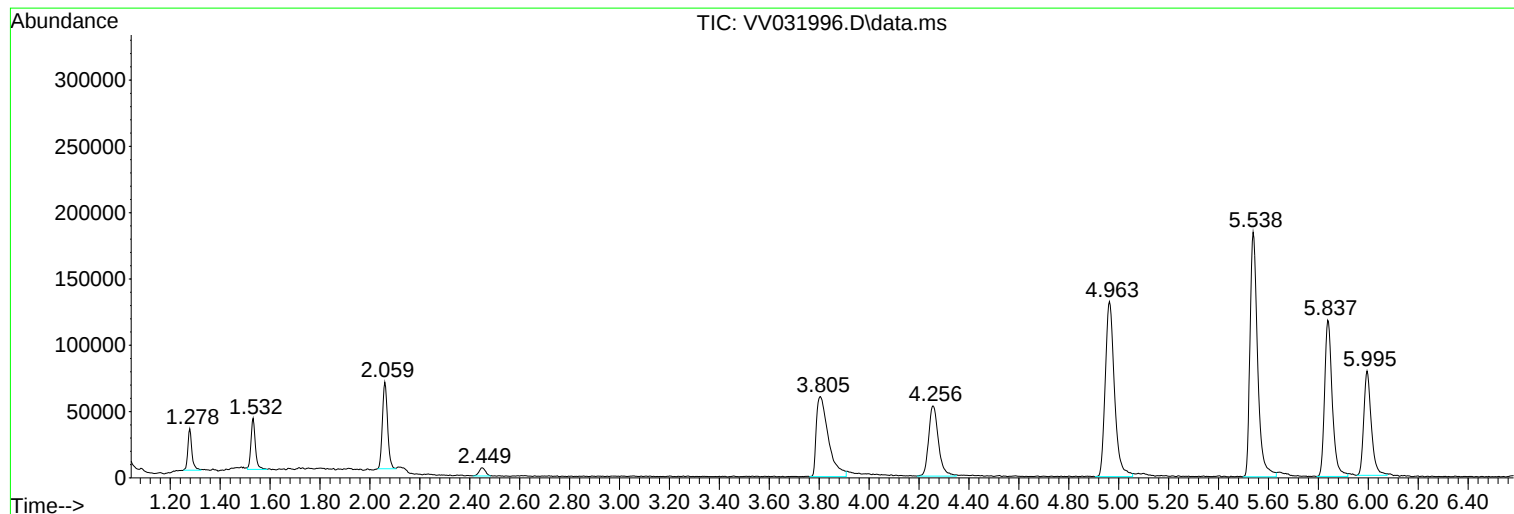

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031996.D
Acq On : 09 Sep 2023 13:26
Operator : SY/MD
Sample : 04267-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031996.D
Acq On : 09 Sep 2023 13:26
Operator : SY/MD
Sample : 04267-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc