

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV031998.D
 Acq On : 09 Sep 2023 14:15
 Operator : SY/MD
 Sample : 04267-13DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4D7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	33592	38216	8.67%	1.025%
2	1.532	146	153	167	rVB	42365	51264	11.63%	1.375%
3	2.060	307	317	332	rBV	71362	104816	23.78%	2.811%
4	2.449	426	438	449	rBV2	7649	14545	3.30%	0.390%
5	2.709	504	519	541	rBV	102558	214254	48.61%	5.746%
6	3.806	850	860	897	rBV2	65191	222427	50.46%	5.965%
7	4.256	984	1000	1027	rBV2	57504	154742	35.11%	4.150%
8	4.963	1203	1220	1247	rBV2	141913	366721	83.20%	9.835%
9	5.539	1387	1399	1432	rBV	143857	310869	70.53%	8.337%
10	5.844	1481	1494	1512	rBV7	10488	25488	5.78%	0.684%
11	5.995	1528	1541	1561	rBV	85917	183218	41.57%	4.914%
12	6.921	1817	1829	1844	rBV2	30889	62357	14.15%	1.672%
13	7.249	1917	1931	1952	rBV	164093	302539	68.64%	8.114%
14	7.564	2020	2029	2055	rBV	17975	37091	8.42%	0.995%
15	8.031	2163	2174	2209	rBV	215474	440765	100.00%	11.821%
16	8.789	2398	2410	2434	rBV	234503	396022	89.85%	10.621%
17	10.159	2824	2836	2852	rBV	62046	100521	22.81%	2.696%
18	11.191	3142	3157	3180	rBV	264387	428693	97.26%	11.497%
19	11.509	3244	3256	3261	rBV6	2367	4633	1.05%	0.124%
20	11.567	3263	3274	3294	rVB	164006	269583	61.16%	7.230%




Sum of corrected areas: 3728764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031998.D
Acq On : 09 Sep 2023 14:15
Operator : SY/MD
Sample : 04267-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

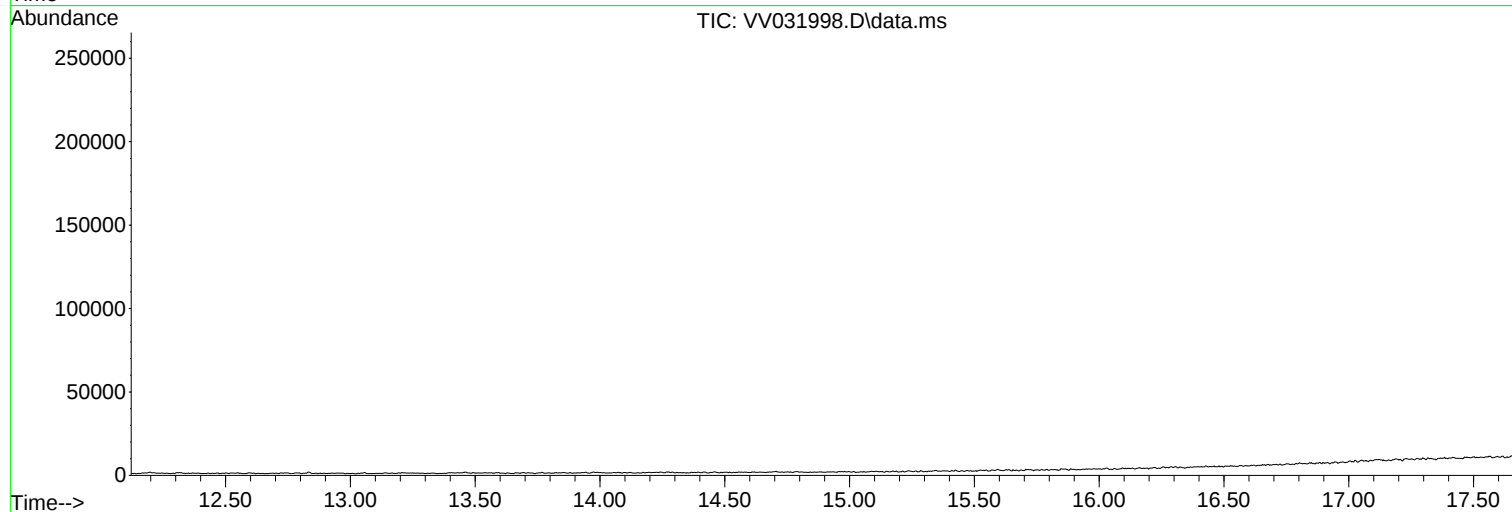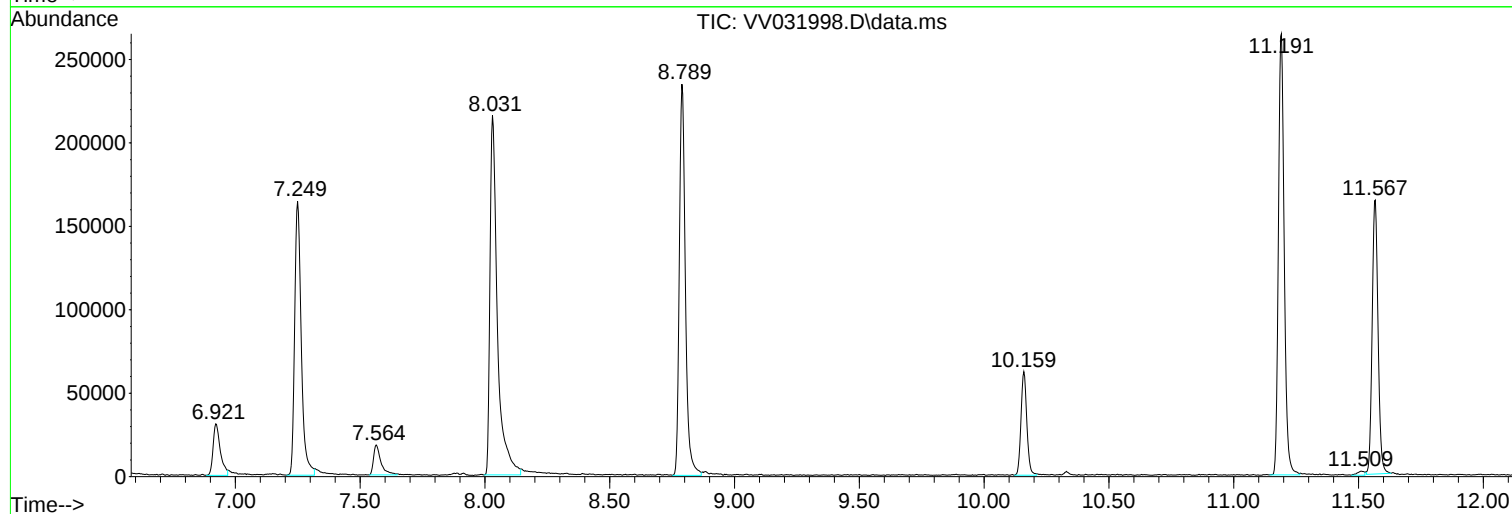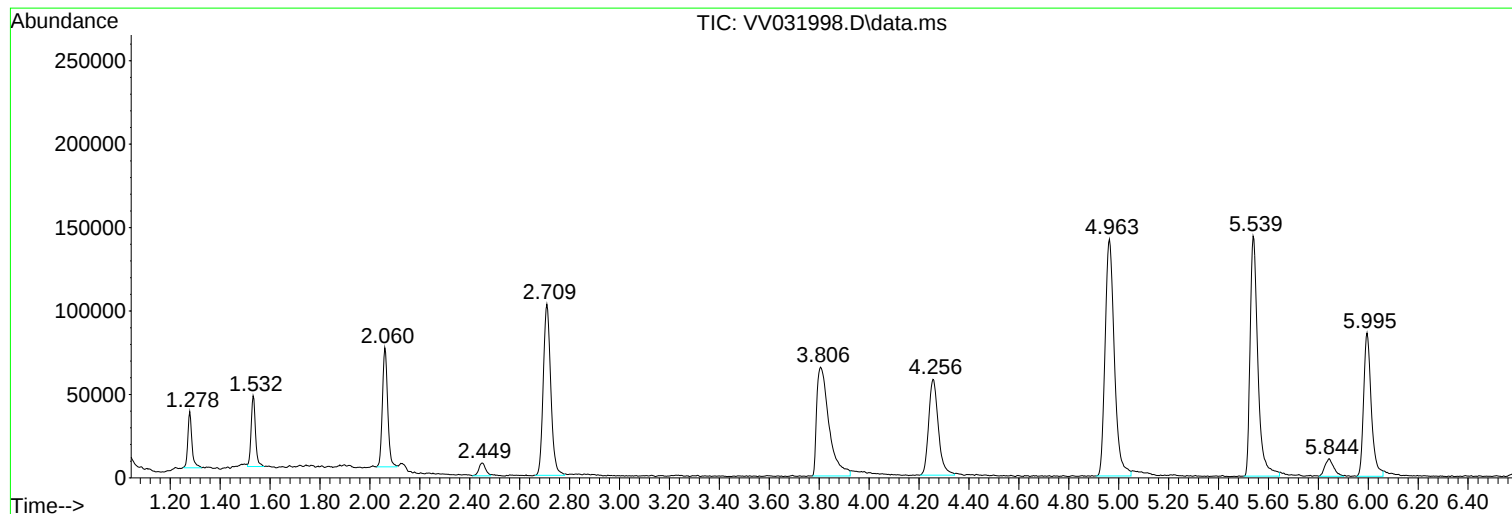

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031998.D
Acq On : 09 Sep 2023 14:15
Operator : SY/MD
Sample : 04267-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031998.D
Acq On : 09 Sep 2023 14:15
Operator : SY/MD
Sample : 04267-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc