

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV031999.D
 Acq On : 09 Sep 2023 14:39
 Operator : SY/MD
 Sample : 04267-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4D7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVV	32724	35863	3.35%	0.767%
2	1.532	146	153	168	rVB	39734	48152	4.50%	1.030%
3	2.060	308	317	332	rBV2	70723	106900	10.00%	2.286%
4	2.706	502	518	540	rBV	515041	1069189	100.00%	22.863%
5	3.815	844	863	900	rBV2	112559	372622	34.85%	7.968%
6	4.256	980	1000	1027	rBV	56320	153481	14.35%	3.282%
7	4.963	1202	1220	1248	rBV3	132853	350189	32.75%	7.488%
8	5.539	1385	1399	1423	rBV2	141020	298982	27.96%	6.393%
9	5.841	1481	1493	1513	rBV3	39311	88417	8.27%	1.891%
10	5.995	1528	1541	1564	rBV2	79443	172845	16.17%	3.696%
11	6.921	1816	1829	1850	rBV2	30009	61316	5.73%	1.311%
12	7.249	1919	1931	1958	rBV	153633	286668	26.81%	6.130%
13	7.564	2018	2029	2046	rBV2	17572	34293	3.21%	0.733%
14	8.030	2165	2174	2211	rBV	213870	421888	39.46%	9.022%
15	8.789	2400	2410	2432	rBV	223644	382477	35.77%	8.179%
16	10.159	2819	2836	2854	rBV	58817	97503	9.12%	2.085%
17	11.191	3146	3157	3178	rBV	260907	416828	38.99%	8.913%
18	11.500	3241	3253	3263	rBV3	9735	21782	2.04%	0.466%
19	11.567	3263	3274	3289	rVB	160172	257014	24.04%	5.496%




Sum of corrected areas: 4676409

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031999.D
Acq On : 09 Sep 2023 14:39
Operator : SY/MD
Sample : 04267-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

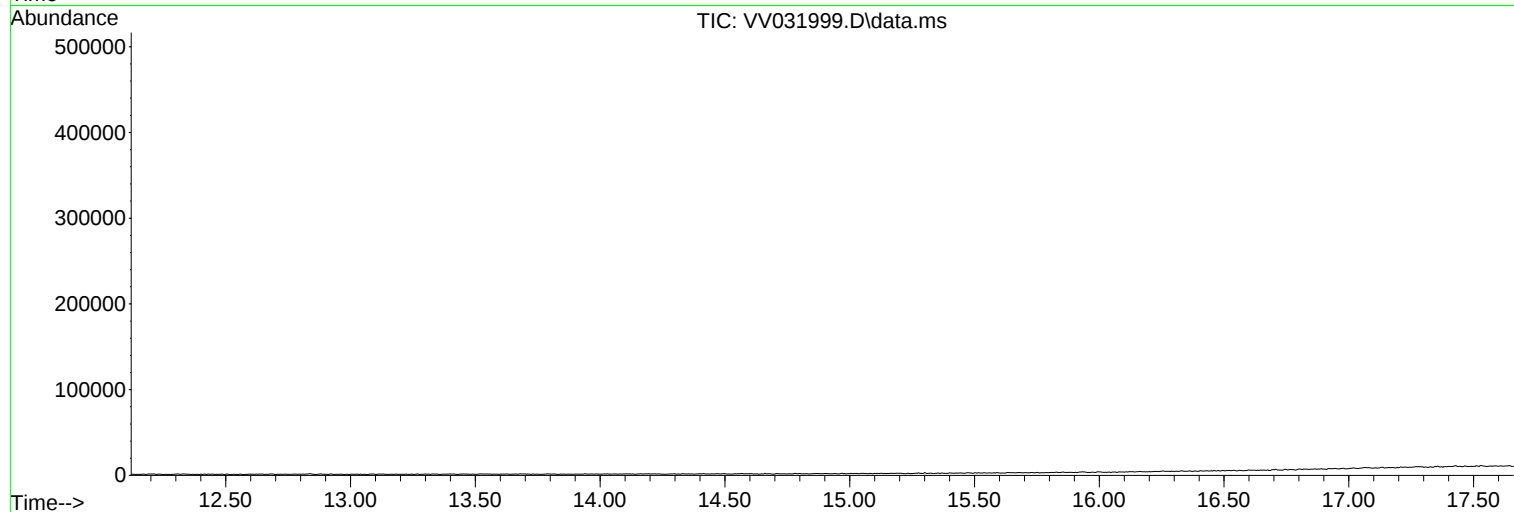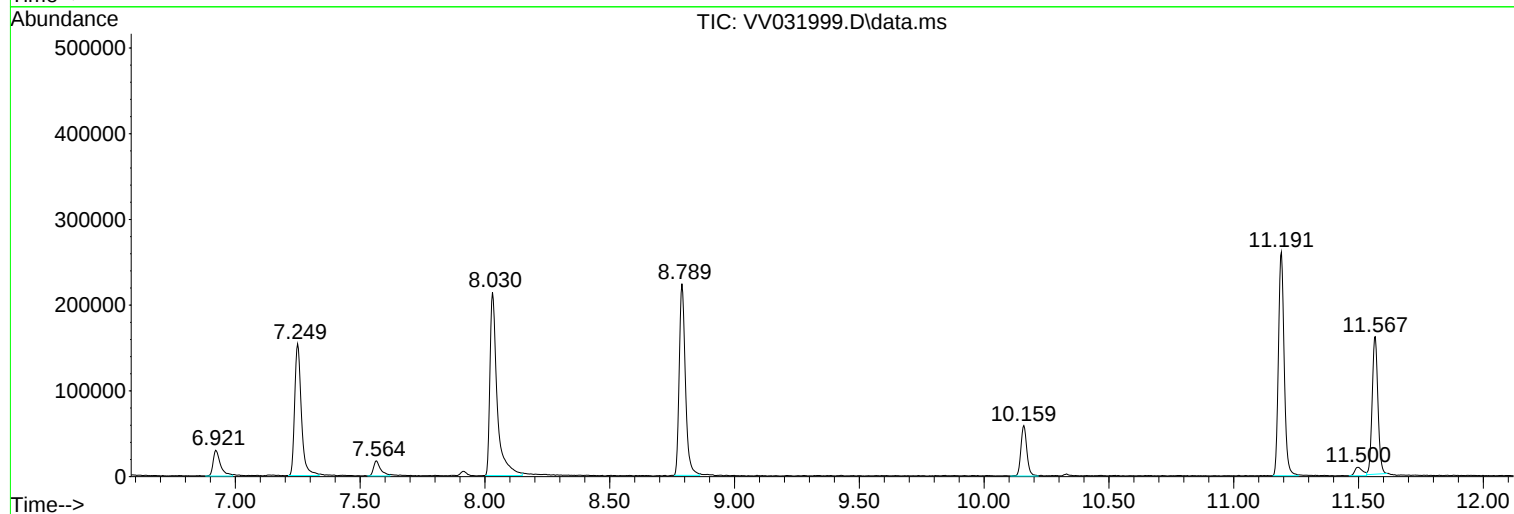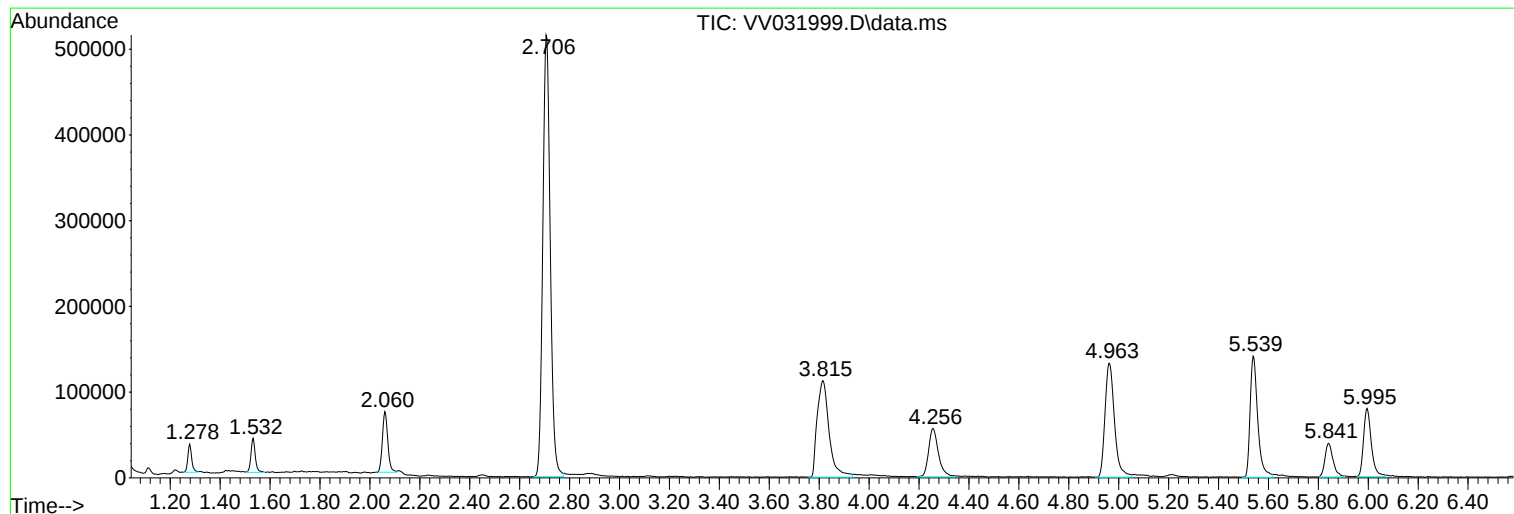

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031999.D
Acq On : 09 Sep 2023 14:39
Operator : SY/MD
Sample : 04267-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031999.D
Acq On : 09 Sep 2023 14:39
Operator : SY/MD
Sample : 04267-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc