

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV032000.D
 Acq On : 09 Sep 2023 15:04
 Operator : SY/MD
 Sample : 04267-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4F0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	86	rBV	34740	39034	8.39%	1.125%
2	1.352	91	97	112	rVB	20708	26632	5.73%	0.767%
3	1.532	146	153	164	rVB	41506	47935	10.30%	1.381%
4	2.060	308	317	330	rBV	73043	105990	22.78%	3.054%
5	3.806	850	860	892	rBV	54625	167760	36.06%	4.835%
6	4.256	982	1000	1023	rBV	59817	155749	33.48%	4.488%
7	4.963	1202	1220	1246	rBV2	145755	375302	80.68%	10.815%
8	5.539	1387	1399	1425	rBV	138016	293177	63.03%	8.449%
9	5.831	1480	1490	1504	rBV5	4334	9343	2.01%	0.269%
10	5.995	1528	1541	1563	rBV	86588	189493	40.74%	5.461%
11	6.921	1817	1829	1847	rBV2	32401	65928	14.17%	1.900%
12	7.249	1920	1931	1958	rBV	168541	308625	66.35%	8.894%
13	7.564	2018	2029	2046	rBV2	18891	35989	7.74%	1.037%
14	8.030	2164	2174	2218	rBV	225614	465175	100.00%	13.405%
15	8.789	2399	2410	2436	rBV	216654	364985	78.46%	10.518%
16	10.159	2823	2836	2853	rBV	62539	101639	21.85%	2.929%
17	11.191	3145	3157	3178	rBV	252703	397767	85.51%	11.463%
18	11.493	3240	3251	3263	rBV3	13409	29710	6.39%	0.856%
19	11.564	3263	3273	3294	rVB	171937	282906	60.82%	8.153%
20	12.300	3494	3502	3511	rBV5	4110	6914	1.49%	0.199%




Sum of corrected areas: 3470053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032000.D
Acq On : 09 Sep 2023 15:04
Operator : SY/MD
Sample : 04267-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

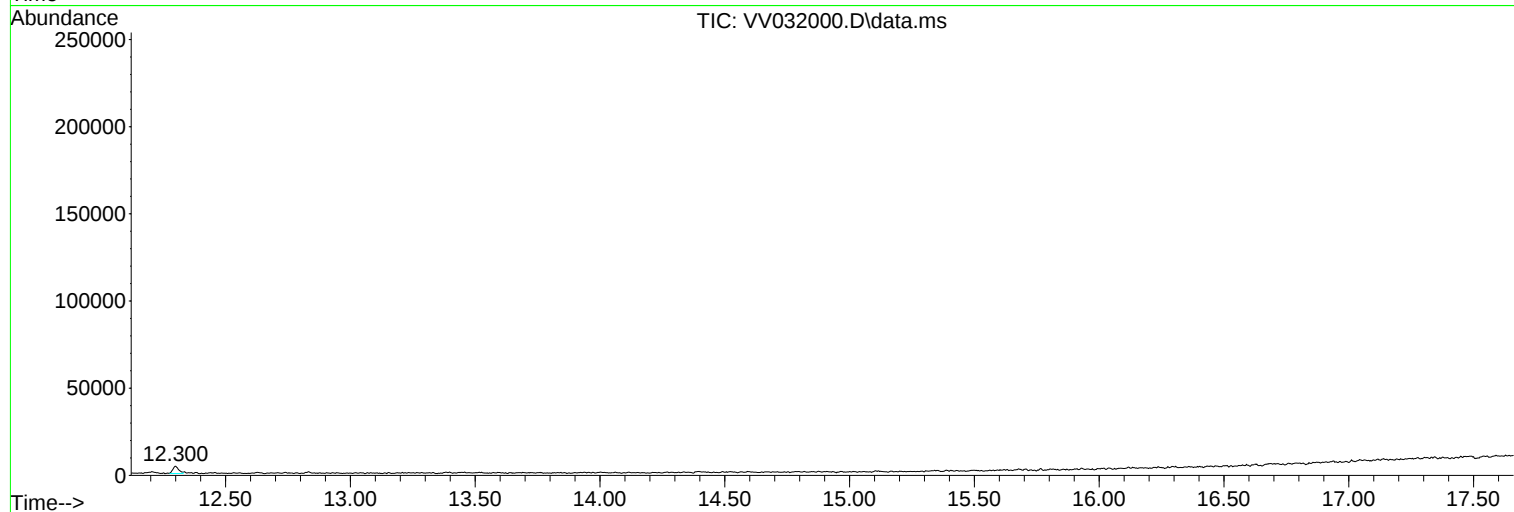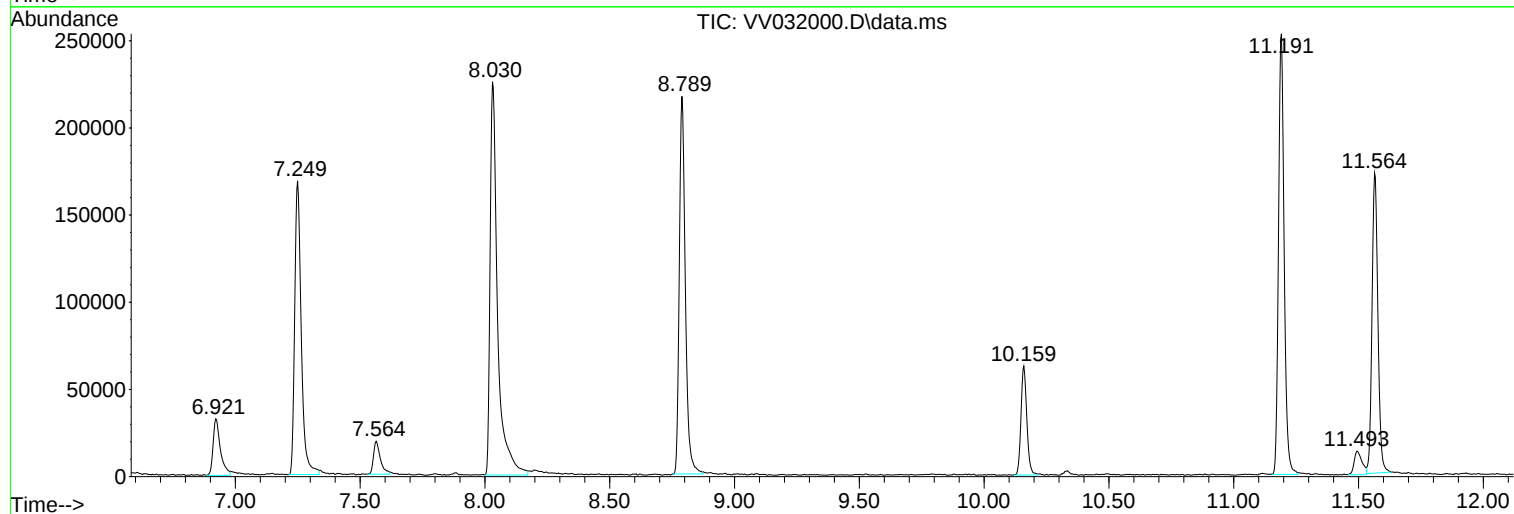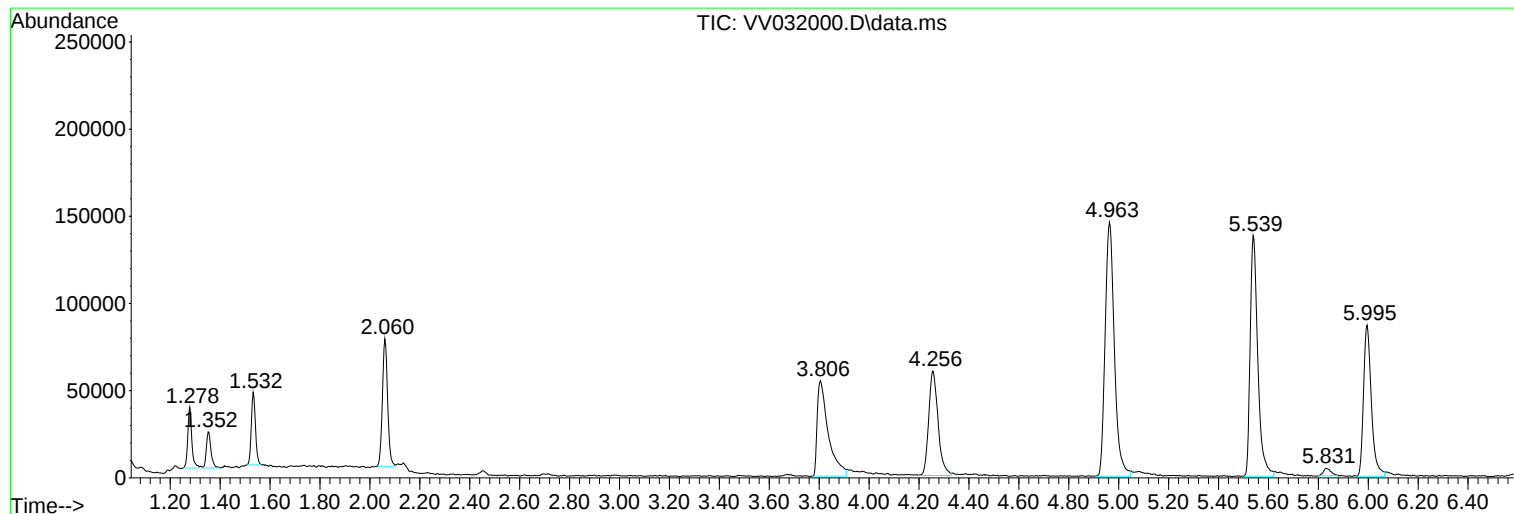

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032000.D
Acq On : 09 Sep 2023 15:04
Operator : SY/MD
Sample : 04267-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032000.D
Acq On : 09 Sep 2023 15:04
Operator : SY/MD
Sample : 04267-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
