

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV032002.D
 Acq On : 09 Sep 2023 15:53
 Operator : SY/MD
 Sample : 04286-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4E0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	35	41	48	rBV	7387	7008	1.52%	0.202%
2	1.278	68	74	85	rVB	34972	36677	7.95%	1.057%
3	1.532	146	153	164	rVB	41337	48658	10.54%	1.402%
4	2.060	308	317	331	rBV	70950	103238	22.37%	2.976%
5	3.799	848	858	890	rBV	57880	167745	36.35%	4.835%
6	4.256	984	1000	1024	rBV	59927	162258	35.16%	4.677%
7	4.963	1202	1220	1241	rBV2	142813	367684	79.67%	10.598%
8	5.539	1386	1399	1423	rBV	137959	292125	63.30%	8.420%
9	5.841	1480	1493	1508	rVB	5564	13621	2.95%	0.393%
10	5.995	1529	1541	1562	rBV	85747	187143	40.55%	5.394%
11	6.921	1818	1829	1853	rBV2	30945	64987	14.08%	1.873%
12	7.249	1920	1931	1965	rBV	167310	309858	67.14%	8.931%
13	7.564	2017	2029	2055	rBV2	18008	37692	8.17%	1.086%
14	7.911	2128	2137	2149	rVB2	10804	18954	4.11%	0.546%
15	8.030	2163	2174	2216	rBV	227763	461484	100.00%	13.301%
16	8.789	2399	2410	2436	rBV	219642	375774	81.43%	10.831%
17	10.159	2825	2836	2853	rBV	62596	101231	21.94%	2.918%
18	10.329	2881	2889	2898	rBV4	3157	4869	1.06%	0.140%
19	11.191	3146	3157	3180	rBV	254546	405201	87.80%	11.679%
20	11.496	3243	3252	3262	rBV3	8948	19668	4.26%	0.567%
21	11.564	3262	3273	3299	rVB	173112	283572	61.45%	8.173%




Sum of corrected areas: 3469447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032002.D
Acq On : 09 Sep 2023 15:53
Operator : SY/MD
Sample : 04286-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

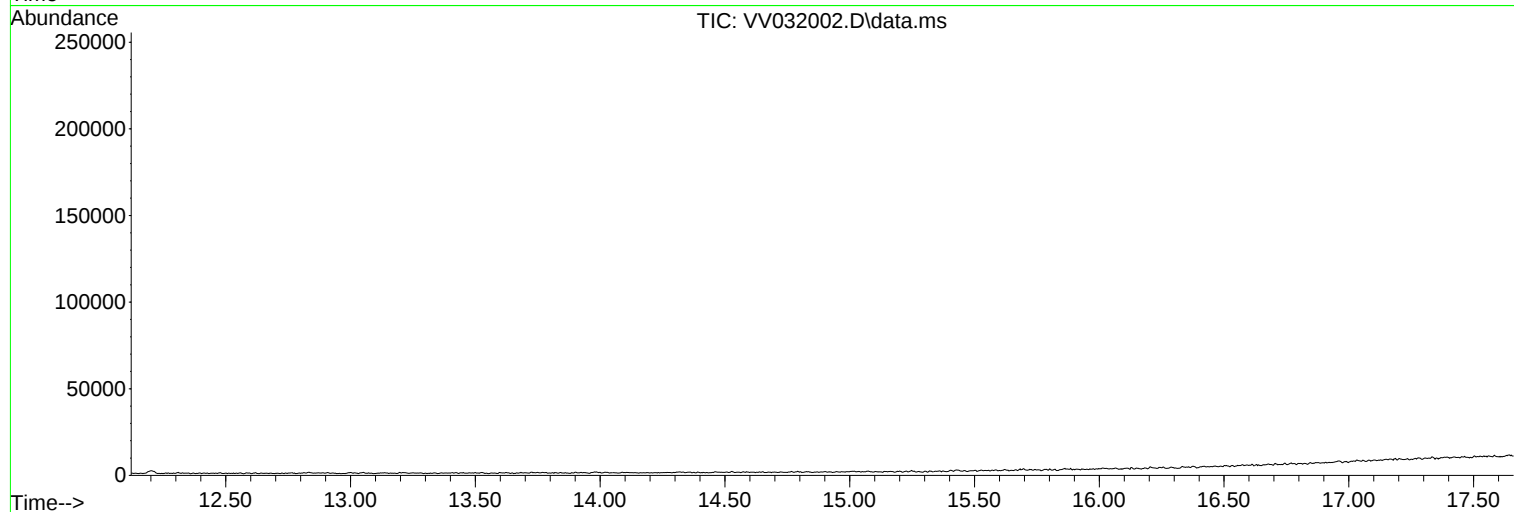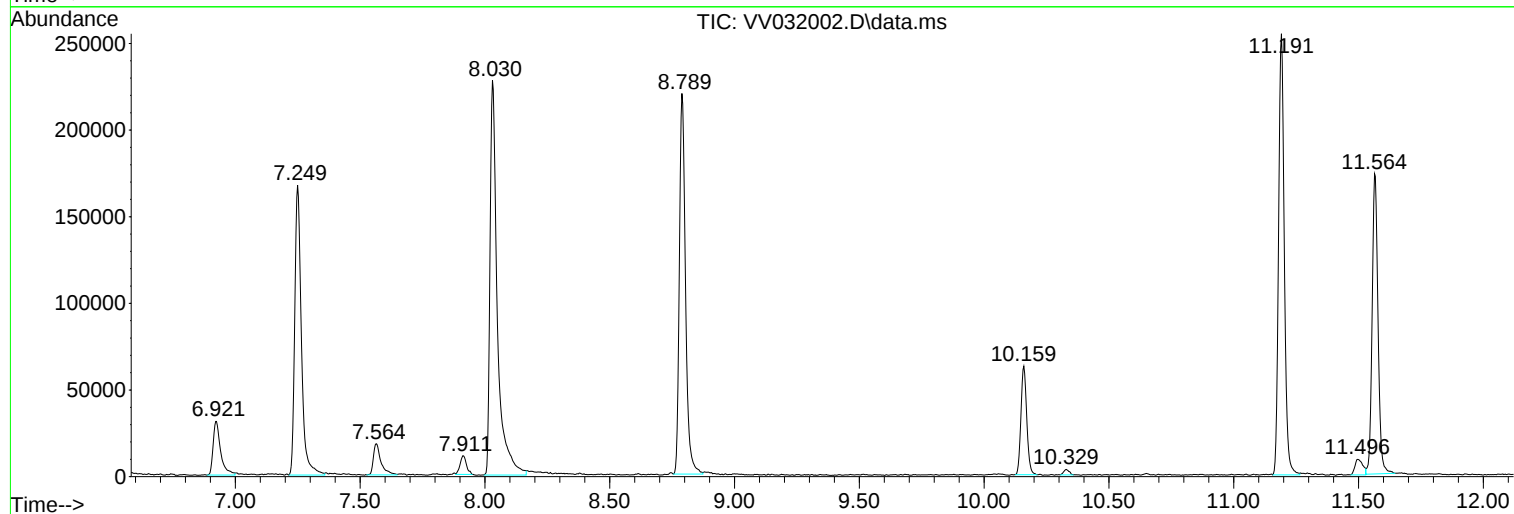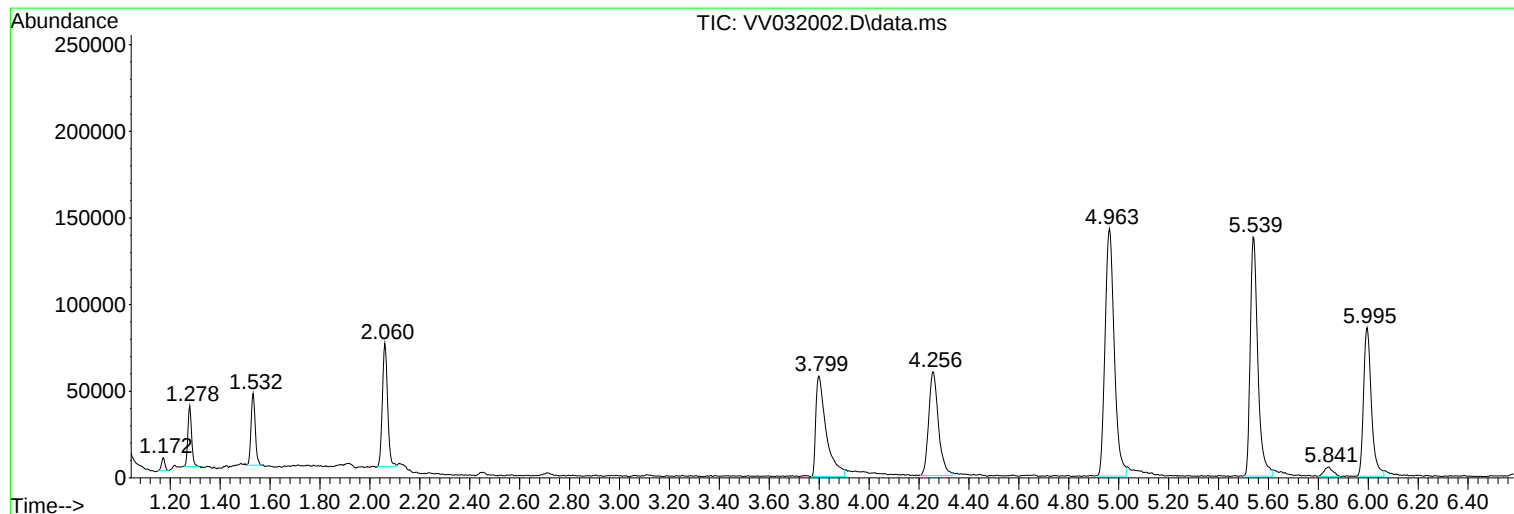

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032002.D
Acq On : 09 Sep 2023 15:53
Operator : SY/MD
Sample : 04286-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032002.D
Acq On : 09 Sep 2023 15:53
Operator : SY/MD
Sample : 04286-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4E0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------