

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV032006.D
 Acq On : 09 Sep 2023 17:31
 Operator : SY/MD
 Sample : 04307-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4J9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	61	rBV5	4329	5995	1.35%	0.166%
2	1.278	68	74	88	rVB	33522	37292	8.40%	1.032%
3	1.532	146	153	164	rVB	39707	45218	10.18%	1.252%
4	2.060	307	317	328	rBV	67537	99081	22.31%	2.743%
5	3.809	851	861	895	rBV	50114	165225	37.21%	4.574%
6	4.256	985	1000	1024	rBV2	56454	153368	34.54%	4.245%
7	4.741	1136	1151	1169	rBV2	38540	91601	20.63%	2.536%
8	4.963	1204	1220	1244	rBV2	134406	349919	78.80%	9.686%
9	5.539	1388	1399	1425	rBV	145157	305836	68.87%	8.466%
10	5.838	1481	1492	1517	rVB10	6133	15891	3.58%	0.440%
11	5.995	1527	1541	1564	rBV	82710	178033	40.09%	4.928%
12	6.921	1819	1829	1858	rBV	28621	61143	13.77%	1.693%
13	7.249	1920	1931	1956	rBV	160183	289092	65.10%	8.002%
14	7.564	2019	2029	2047	rBV2	17083	34281	7.72%	0.949%
15	7.908	2122	2136	2153	rBV	86295	151507	34.12%	4.194%
16	8.031	2164	2174	2218	rBV	215232	444061	100.00%	12.292%
17	8.789	2398	2410	2432	rBV	228887	389598	87.74%	10.785%
18	10.159	2823	2836	2849	rBV	61198	97238	21.90%	2.692%
19	11.191	3146	3157	3181	rBV	267837	425137	95.74%	11.768%
20	11.506	3244	3255	3262	rBV6	4838	10866	2.45%	0.301%
21	11.564	3262	3273	3293	rVB	161992	262174	59.04%	7.257%




Sum of corrected areas: 3612556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032006.D
Acq On : 09 Sep 2023 17:31
Operator : SY/MD
Sample : 04307-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

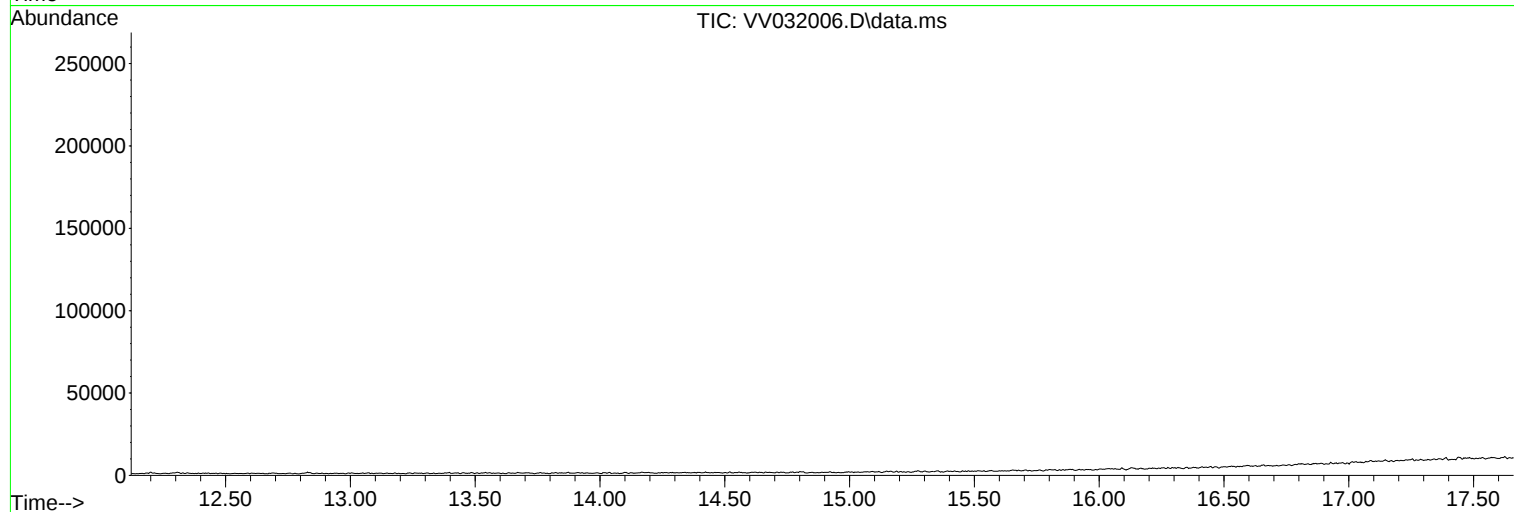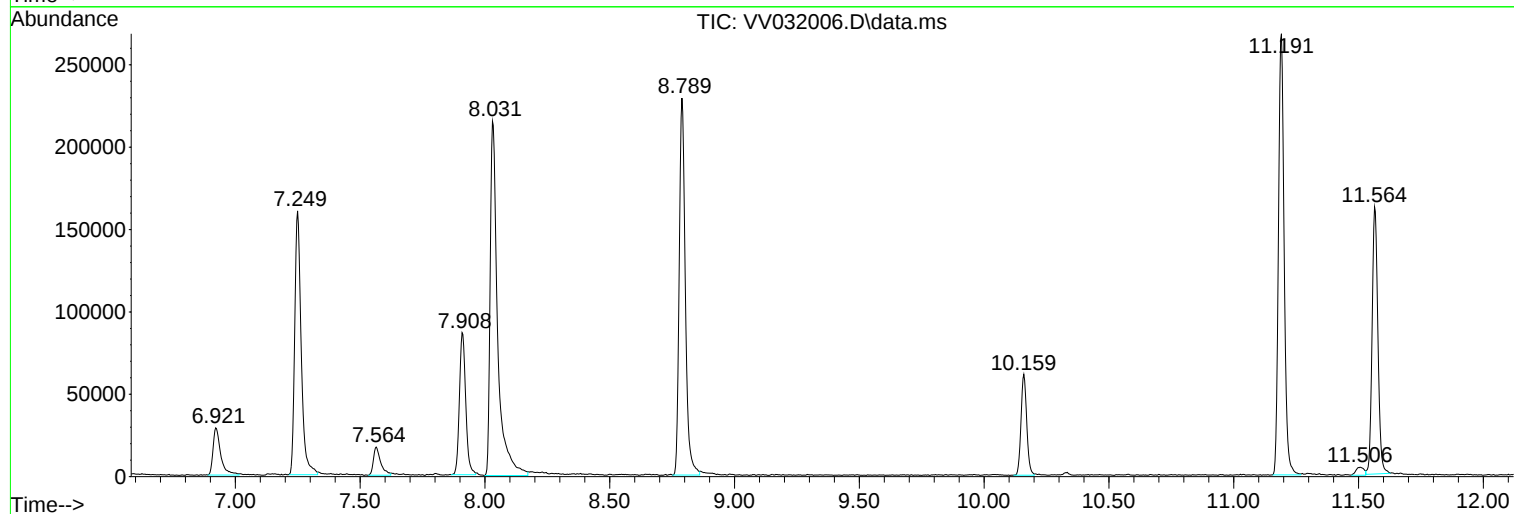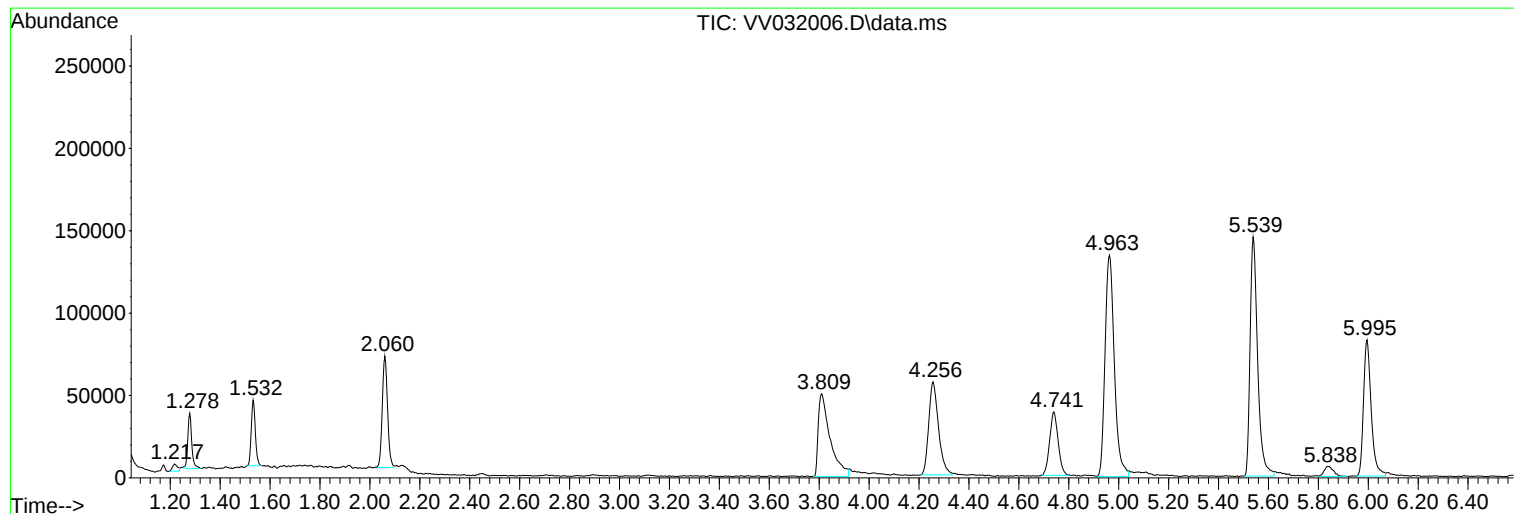

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032006.D
Acq On : 09 Sep 2023 17:31
Operator : SY/MD
Sample : 04307-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032006.D
Acq On : 09 Sep 2023 17:31
Operator : SY/MD
Sample : 04307-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------