

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV032007.D
 Acq On : 09 Sep 2023 17:54
 Operator : SY/MD
 Sample : 04307-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4K0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	34	41	48	rBV	16431	16204	3.64%	0.460%
2	1.278	68	74	83	rVB	33117	34415	7.73%	0.976%
3	1.532	146	153	165	rBV	40690	47005	10.56%	1.333%
4	2.060	304	317	331	rBV	69537	105939	23.79%	3.005%
5	3.799	849	858	892	rBV	59463	175198	39.35%	4.969%
6	4.259	985	1001	1030	rBV2	57358	156817	35.22%	4.448%
7	4.741	1135	1151	1170	rBV2	18271	44702	10.04%	1.268%
8	4.963	1206	1220	1242	rBV3	139075	357257	80.24%	10.132%
9	5.539	1385	1399	1421	rBV	137564	292770	65.76%	8.303%
10	5.844	1479	1494	1511	rBV7	12389	30411	6.83%	0.863%
11	5.995	1527	1541	1571	rBV	83686	186516	41.89%	5.290%
12	6.924	1819	1830	1853	rBV2	30244	65270	14.66%	1.851%
13	7.249	1920	1931	1959	rBV	161894	298409	67.02%	8.463%
14	7.564	2021	2029	2051	rBV	17814	36462	8.19%	1.034%
15	7.911	2125	2137	2158	rVB	44942	81575	18.32%	2.314%
16	8.030	2164	2174	2218	rBV	220417	445225	100.00%	12.627%
17	8.789	2400	2410	2436	rBV	218303	375384	84.31%	10.647%
18	10.159	2825	2836	2852	rBV2	59567	97137	21.82%	2.755%
19	11.191	3146	3157	3181	rBV	260760	407628	91.56%	11.561%
20	11.503	3244	3254	3262	rBV6	3895	8558	1.92%	0.243%
21	11.564	3263	3273	3293	rVB	162015	262987	59.07%	7.459%




Sum of corrected areas: 3525869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032007.D
Acq On : 09 Sep 2023 17:54
Operator : SY/MD
Sample : 04307-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

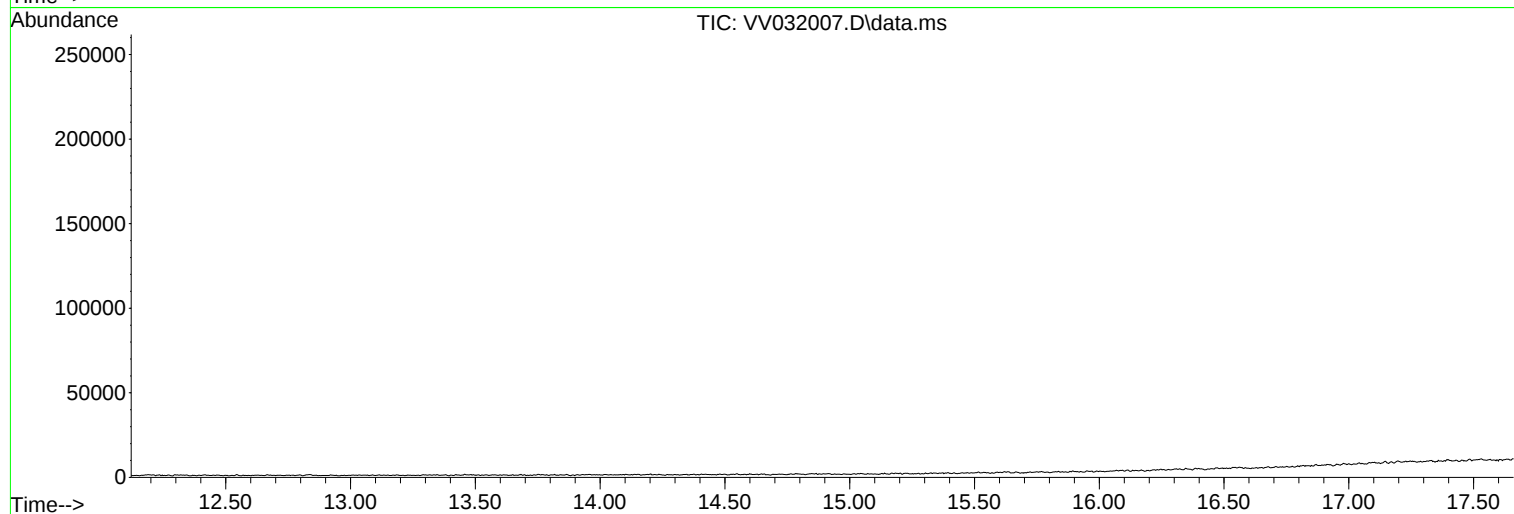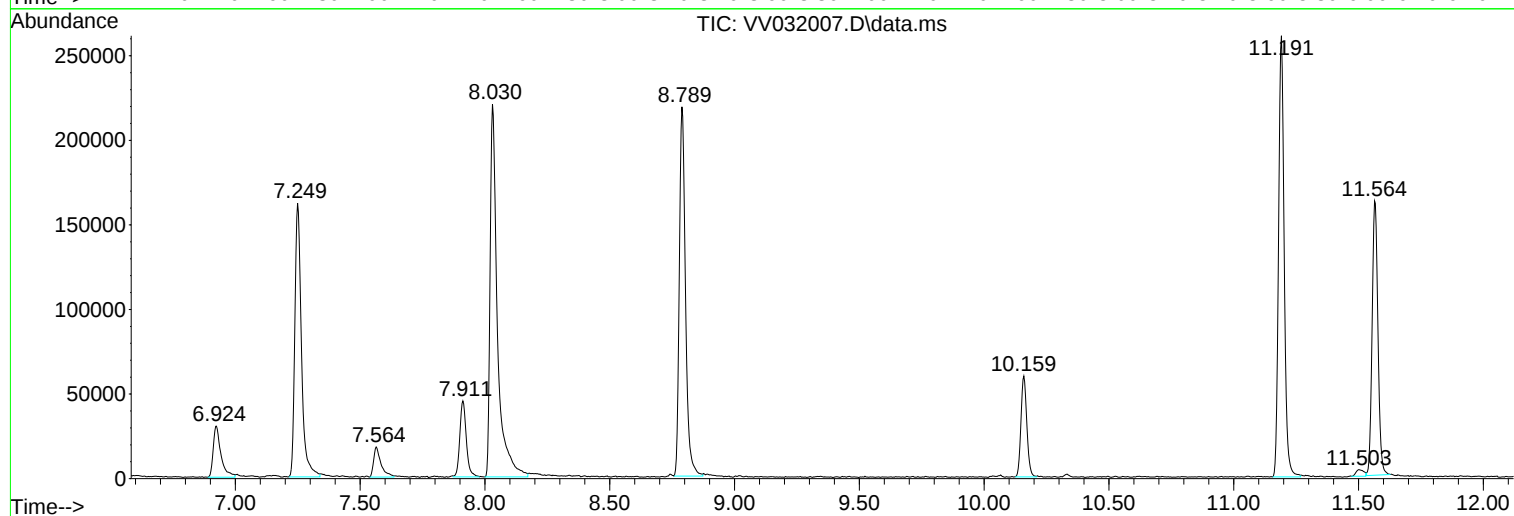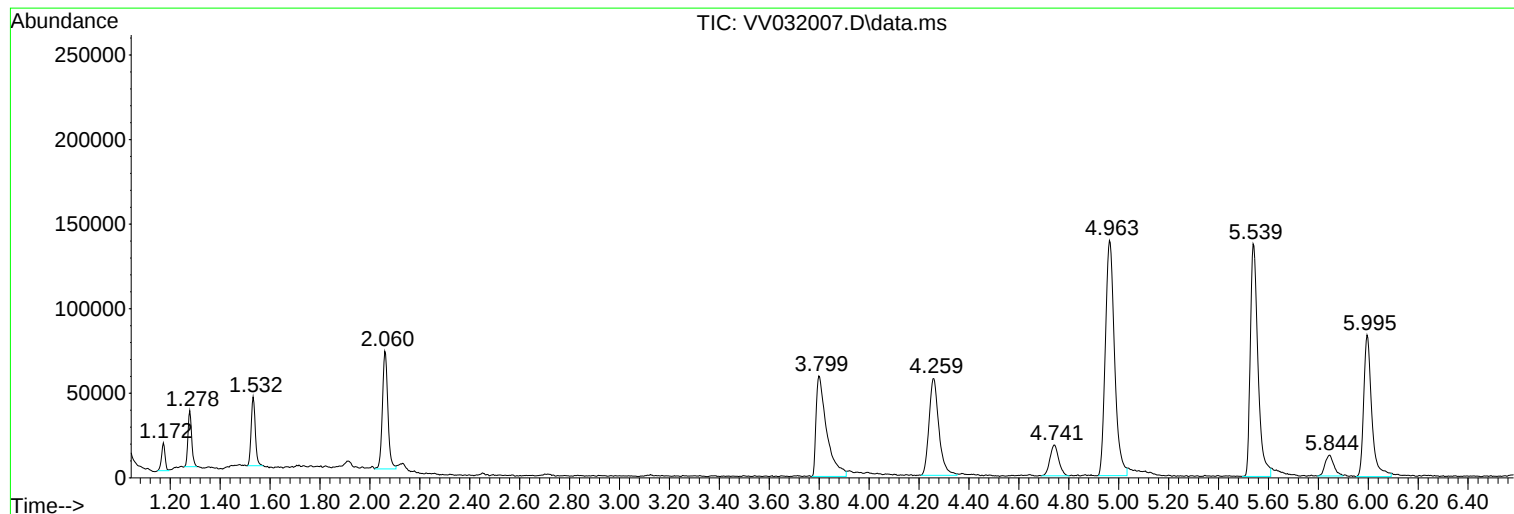

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032007.D
Acq On : 09 Sep 2023 17:54
Operator : SY/MD
Sample : 04307-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032007.D
Acq On : 09 Sep 2023 17:54
Operator : SY/MD
Sample : 04307-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------