

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
 Data File : VV032009.D
 Acq On : 09 Sep 2023 18:43
 Operator : SY/MD
 Sample : 04267-16DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4K2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	30911	32342	7.70%	0.909%
2	1.532	146	153	167	rVB	39769	47893	11.40%	1.346%
3	2.060	308	317	330	rBV	64853	94702	22.55%	2.662%
4	2.449	431	438	451	rVB4	4926	8556	2.04%	0.241%
5	2.709	501	519	542	rBV	125246	264371	62.95%	7.432%
6	3.809	848	861	893	rBV2	62023	211191	50.29%	5.937%
7	4.256	984	1000	1023	rBV3	52703	141645	33.73%	3.982%
8	4.963	1204	1220	1244	rBV2	129049	331016	78.82%	9.305%
9	5.539	1387	1399	1424	rBV	143965	304259	72.45%	8.553%
10	5.841	1481	1493	1515	rVB5	11484	28778	6.85%	0.809%
11	5.995	1528	1541	1565	rBV	77928	169134	40.28%	4.755%
12	6.924	1818	1830	1847	rBV	27899	56602	13.48%	1.591%
13	7.249	1918	1931	1955	rBV	147152	273541	65.14%	7.690%
14	7.564	2020	2029	2048	rBV2	15648	32941	7.84%	0.926%
15	8.030	2165	2174	2220	rBV	197734	406905	96.90%	11.439%
16	8.789	2398	2410	2431	rBV	228481	385800	91.87%	10.845%
17	10.159	2824	2836	2851	rBV	56202	89262	21.26%	2.509%
18	11.191	3144	3157	3174	rBV	265224	419943	100.00%	11.805%
19	11.503	3244	3254	3263	rBV5	6461	13448	3.20%	0.378%
20	11.564	3263	3273	3291	rVB	152829	244994	58.34%	6.887%




Sum of corrected areas: 3557323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032009.D
Acq On : 09 Sep 2023 18:43
Operator : SY/MD
Sample : 04267-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

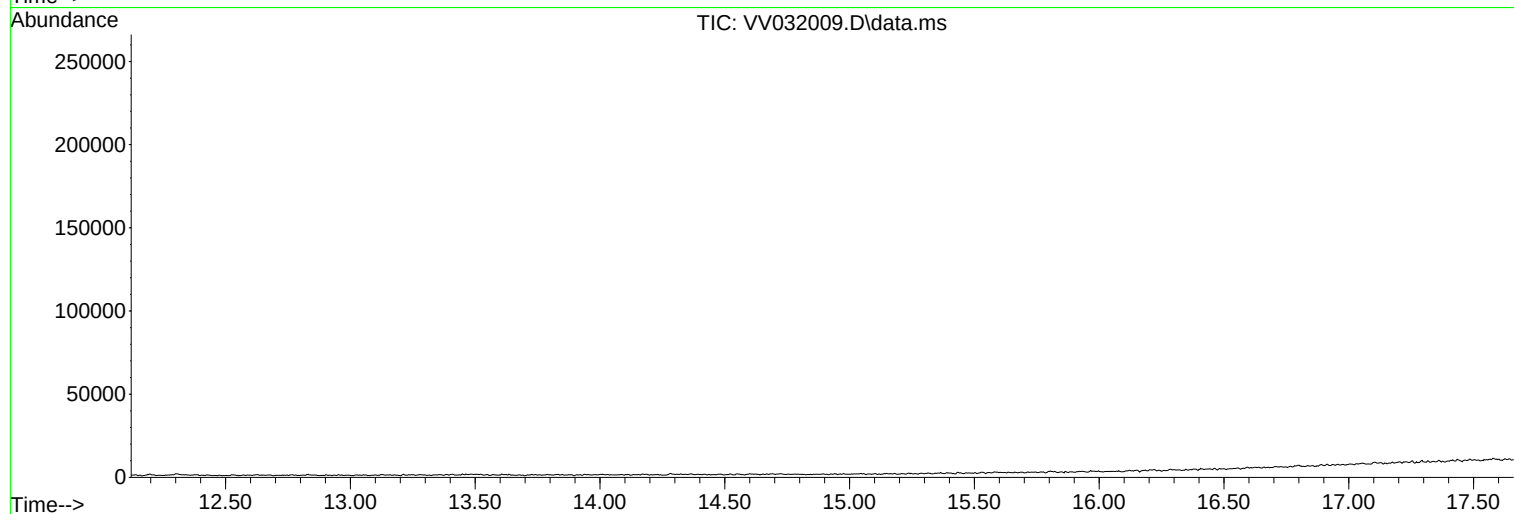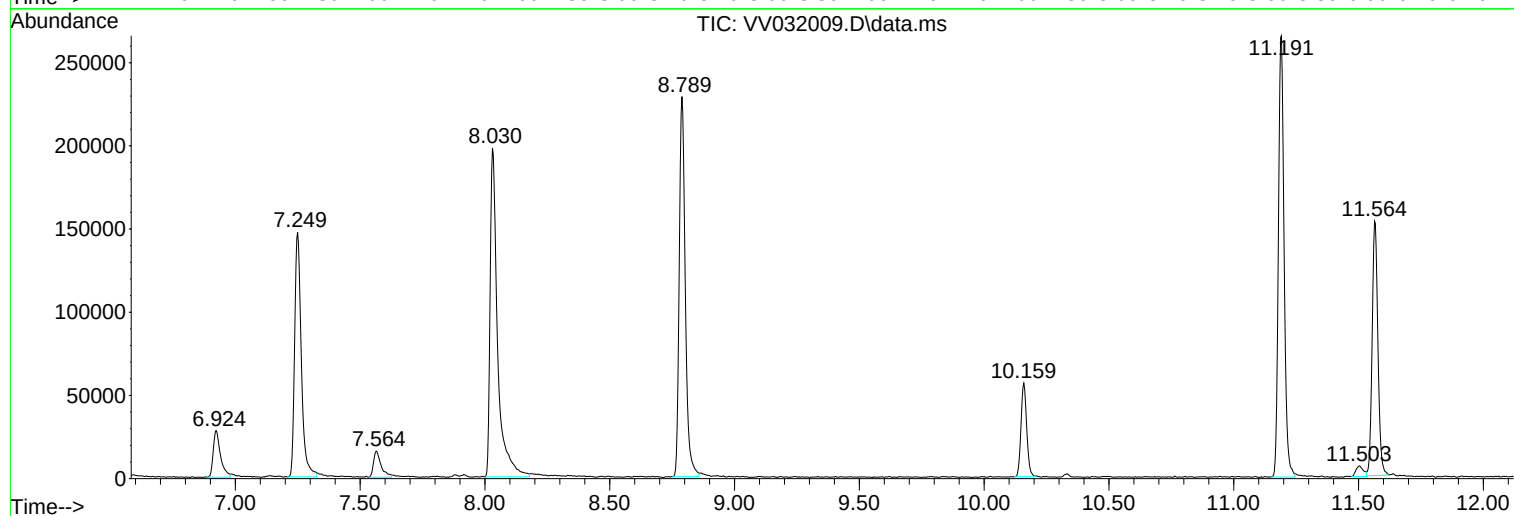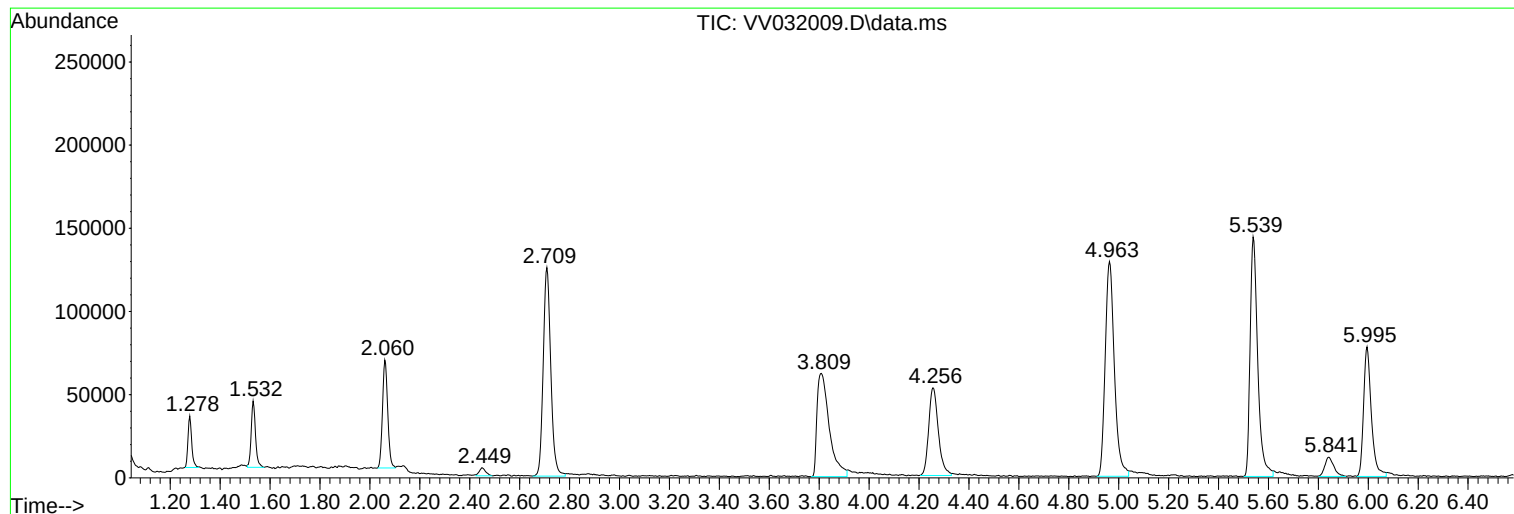

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032009.D
Acq On : 09 Sep 2023 18:43
Operator : SY/MD
Sample : 04267-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV032009.D
Acq On : 09 Sep 2023 18:43
Operator : SY/MD
Sample : 04267-16DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc