
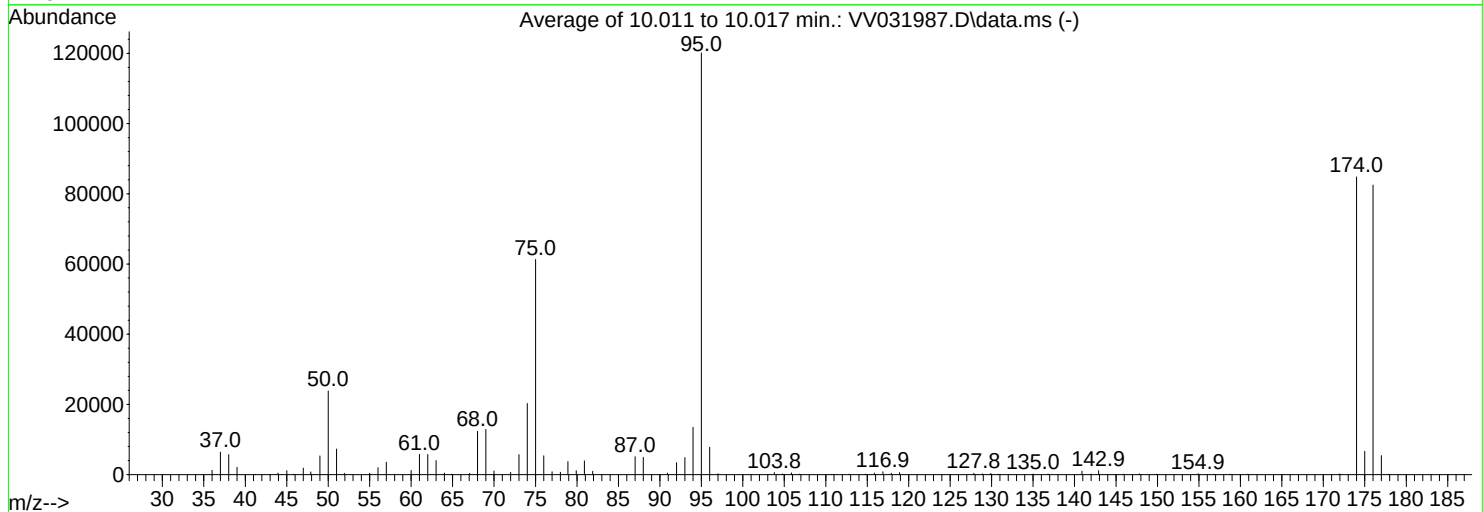


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090923\
Data File : VV031987.D
Acq On : 09 Sep 2023 08:55
Operator : SY/MD
Sample : BFB289
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB289

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 09 21:51:31 2023

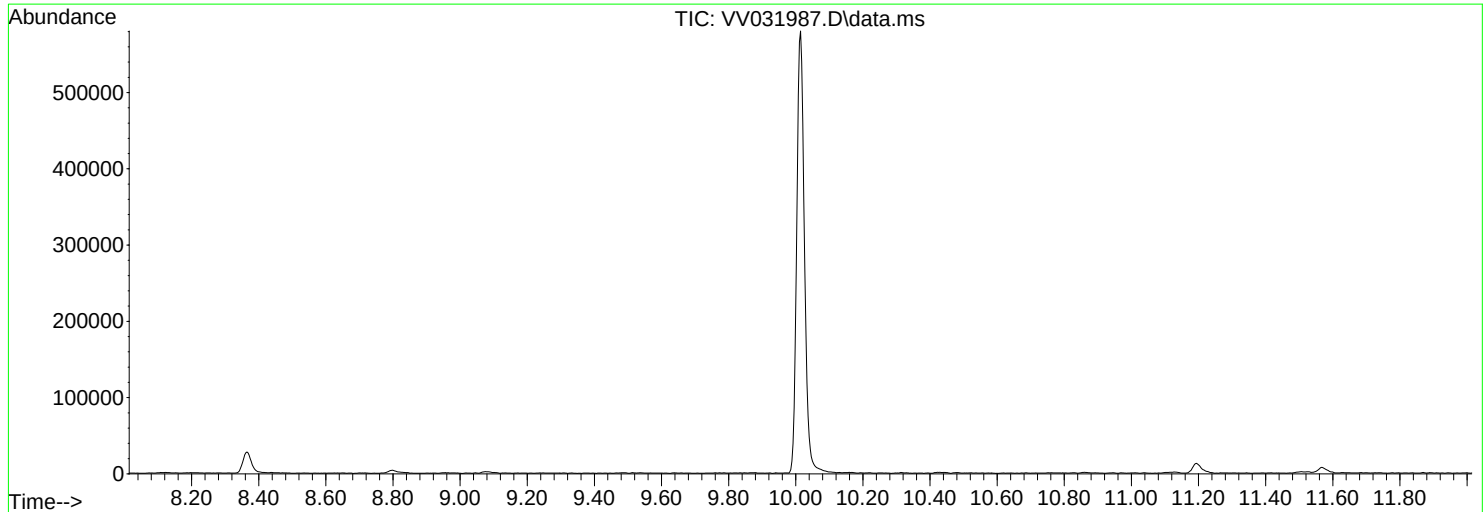

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	23859	PASS
75	95	30	80	51.0	61293	PASS
95	95	100	100	100.0	120147	PASS
96	95	5	9	6.5	7799	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	84821	PASS
175	174	5	9	7.9	6675	PASS
176	174	95	105	97.2	82477	PASS
177	176	5	10	6.6	5412	PASS

m/z	Abundance
39.00	141.0
39.90	257.0
40.90	119.0
42.90	100.0
43.90	608.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	1220.0
37.00	6469.0
38.00	5987.0
39.00	2360.0
39.90	226.0
41.20	114.0
42.90	182.0
44.00	1142.0
45.00	1156.0
45.90	101.0
47.00	1958.0
47.90	814.0
49.00	5451.0
50.00	24520.0
51.00	7627.0
52.00	396.0
55.00	389.0
56.00	2004.0
57.00	3637.0
58.00	178.0
60.00	1282.0
61.00	5847.0
62.00	5768.0
63.00	4229.0
64.00	480.0
64.90	157.0
67.00	392.0
68.00	12814.0
69.00	13000.0
70.00	1047.0
71.00	122.0
72.00	672.0
73.00	5846.0
74.00	20752.0
75.00	62512.0
76.00	5667.0
77.00	863.0
78.00	655.0
78.90	3783.0
79.90	1187.0
80.90	4022.0
81.90	977.0
87.00	5068.0
88.00	4929.0
90.90	468.0
92.00	3380.0
93.00	4843.0
94.00	13677.0
95.00	121384.0
96.00	8075.0
97.00	288.0
103.80	543.0
104.80	219.0
105.90	543.0
106.90	112.0
110.70	118.0
112.90	109.0
114.80	122.0
115.80	404.0
116.90	814.0
117.90	446.0
118.90	612.0
127.80	403.0
128.90	249.0
129.90	409.0
130.80	151.0
135.00	185.0
136.80	182.0
140.90	1061.0
142.10	174.0
142.90	1087.0
144.00	106.0
144.80	101.0
145.90	141.0
147.80	218.0
149.80	117.0
154.90	229.0
156.80	170.0
158.70	147.0
160.90	120.0
171.90	331.0
174.00	83544.0
175.00	6786.0
176.00	80752.0
177.00	5386.0
177.90	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	1272.0
37.00	6590.0
38.00	5879.0
39.00	2331.0
39.90	240.0
40.80	110.0
42.90	166.0
44.00	1086.0
45.00	1138.0
45.80	126.0
47.00	1935.0
47.90	818.0
49.00	5495.0
50.00	24632.0
51.00	7435.0
52.00	364.0
55.00	425.0
56.00	2084.0
57.00	3661.0
58.00	158.0
60.00	1248.0
61.00	5943.0
62.00	5888.0
63.00	4121.0
64.00	503.0
64.80	137.0
67.10	391.0
68.00	12801.0
69.00	13394.0
70.00	1099.0
72.00	641.0
73.00	5853.0
74.00	20808.0
75.00	63232.0
76.00	5493.0
77.00	864.0
78.00	699.0
78.90	3841.0
79.90	1175.0
80.90	4042.0
81.90	972.0
87.00	5275.0
88.00	5031.0
90.90	483.0
92.00	3524.0
93.00	5037.0
94.00	13941.0
95.00	124184.0
96.00	7987.0
97.00	294.0
103.80	606.0
104.80	214.0
105.80	499.0
106.80	144.0
110.60	119.0
111.00	114.0
112.80	125.0
114.80	150.0
115.90	448.0
116.90	900.0
117.90	438.0
118.90	635.0
127.90	426.0
128.90	240.0
129.90	379.0
130.80	161.0
135.00	214.0
136.80	180.0
140.90	1034.0
142.00	187.0
142.90	1182.0
143.90	101.0
144.90	110.0
145.80	123.0
147.80	237.0
149.90	115.0
154.90	266.0
156.80	159.0
158.80	140.0
160.90	156.0
171.90	308.0
174.00	87648.0
175.00	6946.0
176.00	85384.0
177.00	5623.0
177.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	1204.0
37.00	6192.0
38.00	5287.0
39.00	2028.0
40.00	246.0
40.80	109.0
42.90	142.0
44.00	1013.0
45.00	1083.0
45.90	143.0
47.00	1751.0
47.90	712.0
49.00	5062.0
50.00	22424.0
51.00	6856.0
51.90	327.0
55.00	417.0
56.00	1923.0
57.00	3370.0
58.00	141.0
60.00	1083.0
61.00	5534.0
62.00	5559.0
63.00	3718.0
64.00	428.0
64.80	136.0
67.10	350.0
68.00	11447.0
69.00	12269.0
70.00	1069.0
72.00	570.0
73.00	5369.0
74.00	19256.0
75.00	58136.0
76.00	4946.0
77.00	746.0
78.00	657.0
78.90	3597.0
79.90	1069.0
80.90	3635.0
81.90	858.0
82.90	132.0
87.00	5033.0
88.00	4806.0
90.90	449.0
92.00	3353.0
93.00	4811.0
94.00	12864.0
95.00	114872.0
96.00	7334.0
97.00	269.0
103.80	585.0
104.80	191.0
105.80	433.0
106.80	159.0
110.90	122.0
112.70	128.0
114.80	157.0
115.90	478.0
116.90	802.0
117.90	392.0
118.90	600.0
127.90	378.0
128.90	214.0
129.90	339.0
130.80	146.0
135.00	200.0
136.80	168.0
140.90	974.0
141.90	163.0
142.90	1180.0
145.00	107.0
145.80	103.0
147.80	229.0
150.00	122.0
154.90	280.0
156.80	129.0
158.80	130.0
160.90	174.0
172.10	261.0
174.00	83272.0
175.00	6294.0
176.00	81296.0
177.00	5227.0
177.90	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289