

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091019\
 Data File : VV012664.D
 Acq On : 10 Sep 2019 18:42
 Operator : SY/MD
 Sample : K4809-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFDB9

Quant Time: Sep 11 06:58:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 11 05:21:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	359953	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	361639	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	146838	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	104658	4.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.80%
7) Chloroethane-d5	1.58	69	94647	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.13	63	125504	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	3.96	46	349768	59.53	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.06%
24) Chloroform-d	4.40	84	210579	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.08	65	113996	5.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.40%
32) Benzene-d6	5.10	84	387568	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
36) 1,2-Dichloropropane-d6	6.12	67	132900	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	300372	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
43) trans-1,3-Dichloropropene-	7.66	79	40945	4.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.80%
46) 2-Hexanone-d5	8.14	63	159053	44.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.06%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	94434	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	131317	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	21662	6.290 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091019\
Data File : VV012664.D
Acq On : 10 Sep 2019 18:42
Operator : SY/MD
Sample : K4809-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFDB9

Quant Time: Sep 11 06:58:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 11 05:21:41 2019
Response via : Initial Calibration

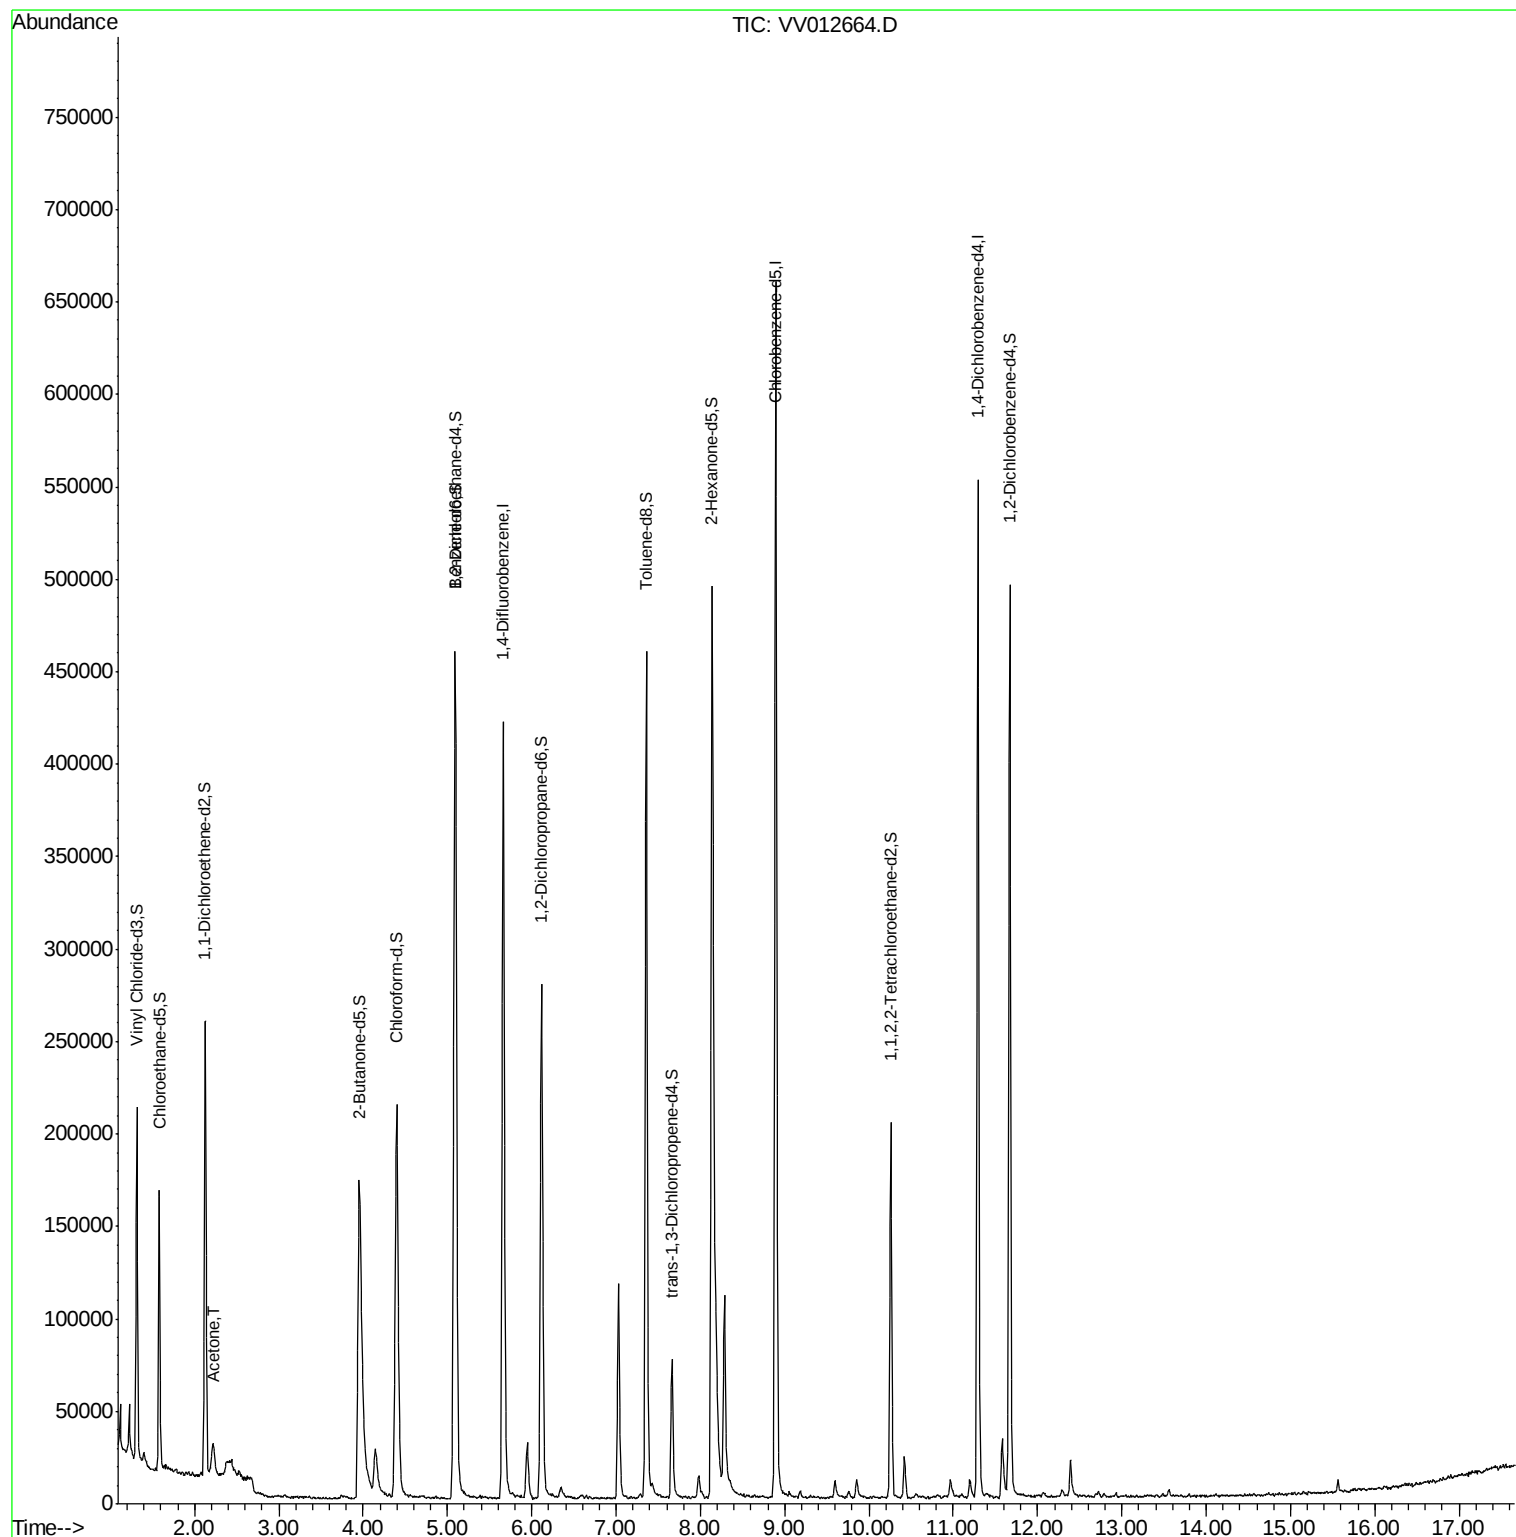

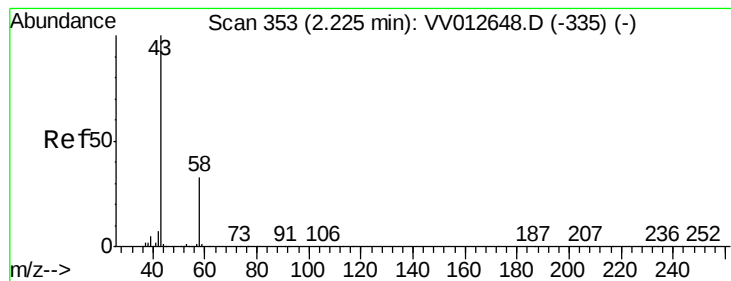

#13

Acetone

Concen: 6.290 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.01 min

Lab File: VV012664.D

Acq: 10 Sep 2019 18:42


Instrument :
MSVOA_V
ClientSampleId :
BFDB9

Tot Ion: 43 Resp: 21662

Ion Ratio Lower Upper

43 100

58 31.0 0.0 67.4

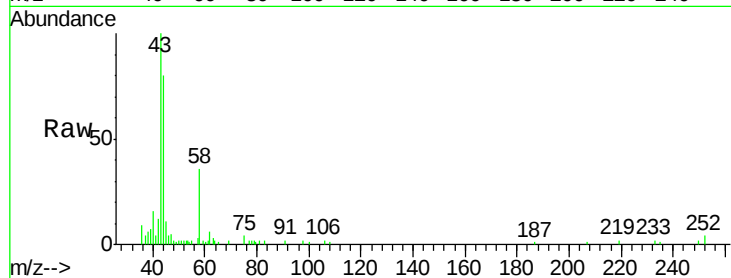

Abundance Ion 43.05 (42.75 to 43.75): VV0
Ion 58.05 (57.75 to 58.75): VV0

