


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091019\
 Data File : VV012647.D
 Acq On : 10 Sep 2019 08:40
 Operator : SY/MD
 Sample : BFB34
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB34

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Sep 12 11:33:34 2019

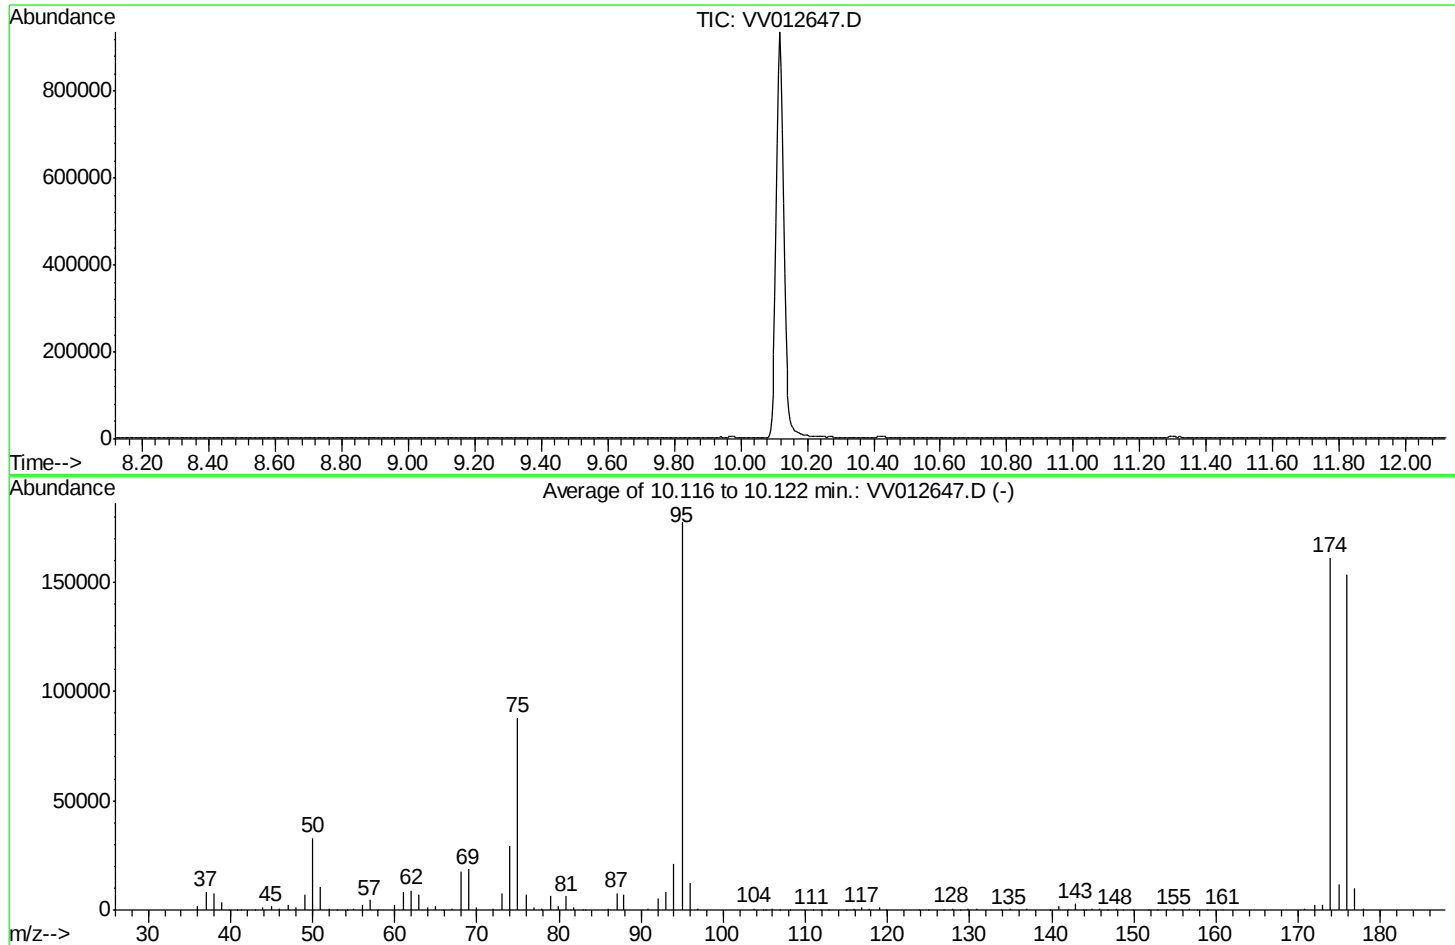

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	32978	PASS
75	95	30	80	49.6	88005	PASS
95	95	100	100	100.0	177301	PASS
96	95	5	9	7.0	12372	PASS
173	174	0.00	2	1.4	2209	PASS
174	95	50	120	90.9	161194	PASS
175	174	5	9	7.2	11546	PASS
176	174	95	101	95.1	153301	PASS
177	176	5	9	6.4	9742	PASS

m/z	Abundance
36.00	1987.0
37.00	8663.0
38.00	8131.0
39.00	3725.0
40.00	1473.0
40.80	238.0
43.00	186.0
44.00	1873.0
45.00	1557.0
46.00	282.0
47.00	2394.0
48.00	1341.0
49.00	7823.0
50.00	34536.0
51.00	10999.0
52.00	577.0
53.00	338.0
54.20	175.0
54.90	434.0
56.00	2656.0
57.00	4892.0
58.00	273.0
60.00	2078.0
61.00	8855.0
62.00	9428.0
63.00	7583.0
64.00	1467.0
65.00	1813.0
65.90	249.0
66.90	462.0
68.00	18104.0
69.00	19520.0
70.00	1352.0
72.00	930.0
73.00	8166.0
74.00	30712.0
75.00	90512.0
76.00	7702.0
77.00	1355.0
78.00	811.0
78.90	6747.0
79.90	1836.0
80.90	6424.0
81.90	1118.0
83.20	161.0
86.00	429.0
87.00	8173.0
87.90	7541.0
90.80	665.0
92.00	5441.0
93.00	8617.0
94.00	21640.0
95.00	182208.0
96.00	12943.0
96.90	416.0
103.80	792.0
104.80	280.0
105.90	681.0
106.90	139.0
109.80	106.0
110.90	250.0
111.90	148.0
112.80	165.0
114.90	179.0
115.90	502.0
116.90	1212.0
117.80	721.0
118.90	1166.0
119.90	120.0
124.90	161.0
126.80	136.0
127.90	720.0
128.80	272.0
129.80	657.0
130.90	456.0
133.80	133.0
134.80	435.0
136.90	339.0
139.80	189.0
140.90	1702.0
142.90	2908.0
143.80	193.0
144.90	948.0
145.80	377.0
146.70	151.0
147.80	387.0
148.70	119.0
149.80	159.0
151.70	137.0
152.80	135.0
153.90	173.0
154.90	516.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

156.80	475.0
157.70	113.0
158.80	229.0
160.80	153.0
170.80	428.0
171.90	2538.0
173.00	2276.0
173.90	162496.0
174.90	12012.0
175.90	154624.0
176.90	10175.0
177.90	339.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	1951.0
37.00	8521.0
38.00	7747.0
39.00	3441.0
40.00	1388.0
40.70	218.0
41.20	139.0
43.00	161.0
44.00	1947.0
45.00	1569.0
46.00	313.0
47.00	2225.0
47.90	1274.0
49.00	7122.0
50.00	33968.0
51.00	10933.0
52.00	525.0
53.00	315.0
54.20	129.0
54.90	459.0
56.00	2466.0
57.00	4820.0
58.00	268.0
60.00	2191.0
61.00	8580.0
62.00	9080.0
63.00	7475.0
64.00	1238.0
65.00	1840.0
65.90	226.0
66.90	492.0
68.00	17744.0
69.00	19296.0
70.00	1370.0
72.00	909.0
73.00	8075.0
74.00	30152.0
75.00	90760.0
76.00	7435.0
76.90	1374.0
77.90	770.0
78.90	6491.0
79.90	1869.0
80.90	6545.0
81.90	1138.0
83.20	150.0
86.00	419.0
87.00	8084.0
87.90	7437.0
90.80	609.0
92.00	5253.0
93.00	8722.0
94.00	21744.0
95.00	182656.0
96.00	12876.0
96.90	332.0
103.80	827.0
105.10	272.0
105.90	753.0
106.90	143.0
110.90	259.0
111.80	132.0
112.80	145.0
114.90	233.0
115.90	537.0
116.90	1117.0
117.80	682.0
118.90	1112.0
119.80	102.0
124.90	139.0
126.80	107.0
127.90	635.0
128.90	290.0
129.80	623.0
130.80	442.0
133.80	182.0
134.90	444.0
136.90	420.0
139.80	155.0
140.90	1811.0
142.90	2996.0
143.90	196.0
144.90	773.0
145.80	323.0
146.70	126.0
147.80	408.0
148.70	164.0
149.90	168.0
151.80	139.0
152.90	118.0
153.80	186.0
154.90	529.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

155.80	111.0
156.80	473.0
158.80	242.0
160.90	180.0
170.80	382.0
171.90	2698.0
173.00	2285.0
173.90	166656.0
174.90	11931.0
175.90	158144.0
176.90	10027.0
177.90	375.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

m/z	Abundance
36.00	1584.0
37.00	7607.0
38.00	6784.0
39.00	3016.0
39.90	1308.0
40.70	183.0
41.20	200.0
43.10	159.0
44.00	2029.0
45.00	1391.0
45.90	388.0
47.00	1930.0
47.90	1198.0
49.00	6078.0
50.00	30432.0
51.00	9717.0
52.00	475.0
53.00	282.0
54.00	123.0
55.00	469.0
56.00	2127.0
57.00	4308.0
58.00	261.0
60.00	1984.0
61.00	7539.0
62.00	7940.0
63.00	6705.0
63.90	995.0
65.00	1762.0
65.90	224.0
66.90	479.0
68.00	16059.0
69.00	17040.0
70.00	1274.0
72.00	774.0
73.00	7338.0
74.00	27120.0
75.00	82744.0
76.00	6812.0
76.90	1202.0
77.80	711.0
78.90	5518.0
79.90	1738.0
80.90	5964.0
81.80	1102.0
82.80	170.0
86.10	329.0
87.00	7261.0
87.90	6963.0
90.90	525.0
92.00	4571.0
93.00	7698.0
94.00	19904.0
95.00	167040.0
96.00	11298.0
97.00	231.0
103.80	739.0
105.10	204.0
105.90	677.0
106.80	132.0
108.10	109.0
110.90	228.0
112.70	140.0
114.90	253.0
115.90	496.0
116.90	1109.0
117.80	578.0
119.00	1036.0
123.80	137.0
127.90	564.0
129.00	283.0
129.90	568.0
130.80	365.0
133.80	161.0
134.90	409.0
136.90	378.0
139.80	111.0
140.90	1761.0
141.90	303.0
142.90	2582.0
144.10	194.0
144.90	706.0
145.90	278.0
147.80	418.0
148.70	173.0
149.80	161.0
150.00	165.0
151.80	110.0
153.00	148.0
153.80	142.0
154.90	500.0
155.80	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

156.80	398.0
158.90	218.0
160.90	177.0
170.80	291.0
172.00	2662.0
173.00	2068.0
173.90	154432.0
174.90	10695.0
175.90	147136.0
176.90	9025.0
177.90	371.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34

Scan 2793 (10.071 min): VV012647.D
BFB34

m/z	Abundance
36.00	185.0
37.70	126.0
39.90	1182.0
43.90	1019.0

Instrument :
MSVOA_V
ClientSampleId :
BFB34