

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091020\
 Data File : VV018176.D
 Acq On : 10 Sep 2020 13:31
 Operator : SY/MD
 Sample : L3957-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWQ7

Quant Time: Sep 11 01:56:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 11 01:30:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	293065	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	291266	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	142407	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	102996	43.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.24%
7) Chloroethane-d5	1.58	69	90534	46.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.64%
11) 1,1-Dichloroethene-d2	2.12	63	151787	34.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.30%
21) 2-Butanone-d5	3.91	46	145777	99.72	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.72%
24) Chloroform-d	4.38	84	193178	46.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.24%
26) 1,2-Dichloroethane-d4	5.06	65	130262	49.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.08%
32) Benzene-d6	5.08	84	394964	47.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.74%
36) 1,2-Dichloropropane-d6	6.09	67	128679	48.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.14%
41) Toluene-d8	7.34	98	351024	46.19	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.38%
43) trans-1,3-Dichloropropene-	7.64	79	61398	45.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.20%
47) 2-Hexanone-d5	8.11	63	104102	103.73	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.73%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	169213	50.89	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.78%
64) 1,2-Dichlorobenzene-d4	11.65	152	151983	51.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.94%


Target Compounds					Ovalue
13) Acetone	2.19	43	1679	1.434 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091020\
Data File : VV018176.D
Acq On : 10 Sep 2020 13:31
Operator : SY/MD
Sample : L3957-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWQ7

Quant Time: Sep 11 01:56:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 11 01:30:09 2020
Response via : Initial Calibration

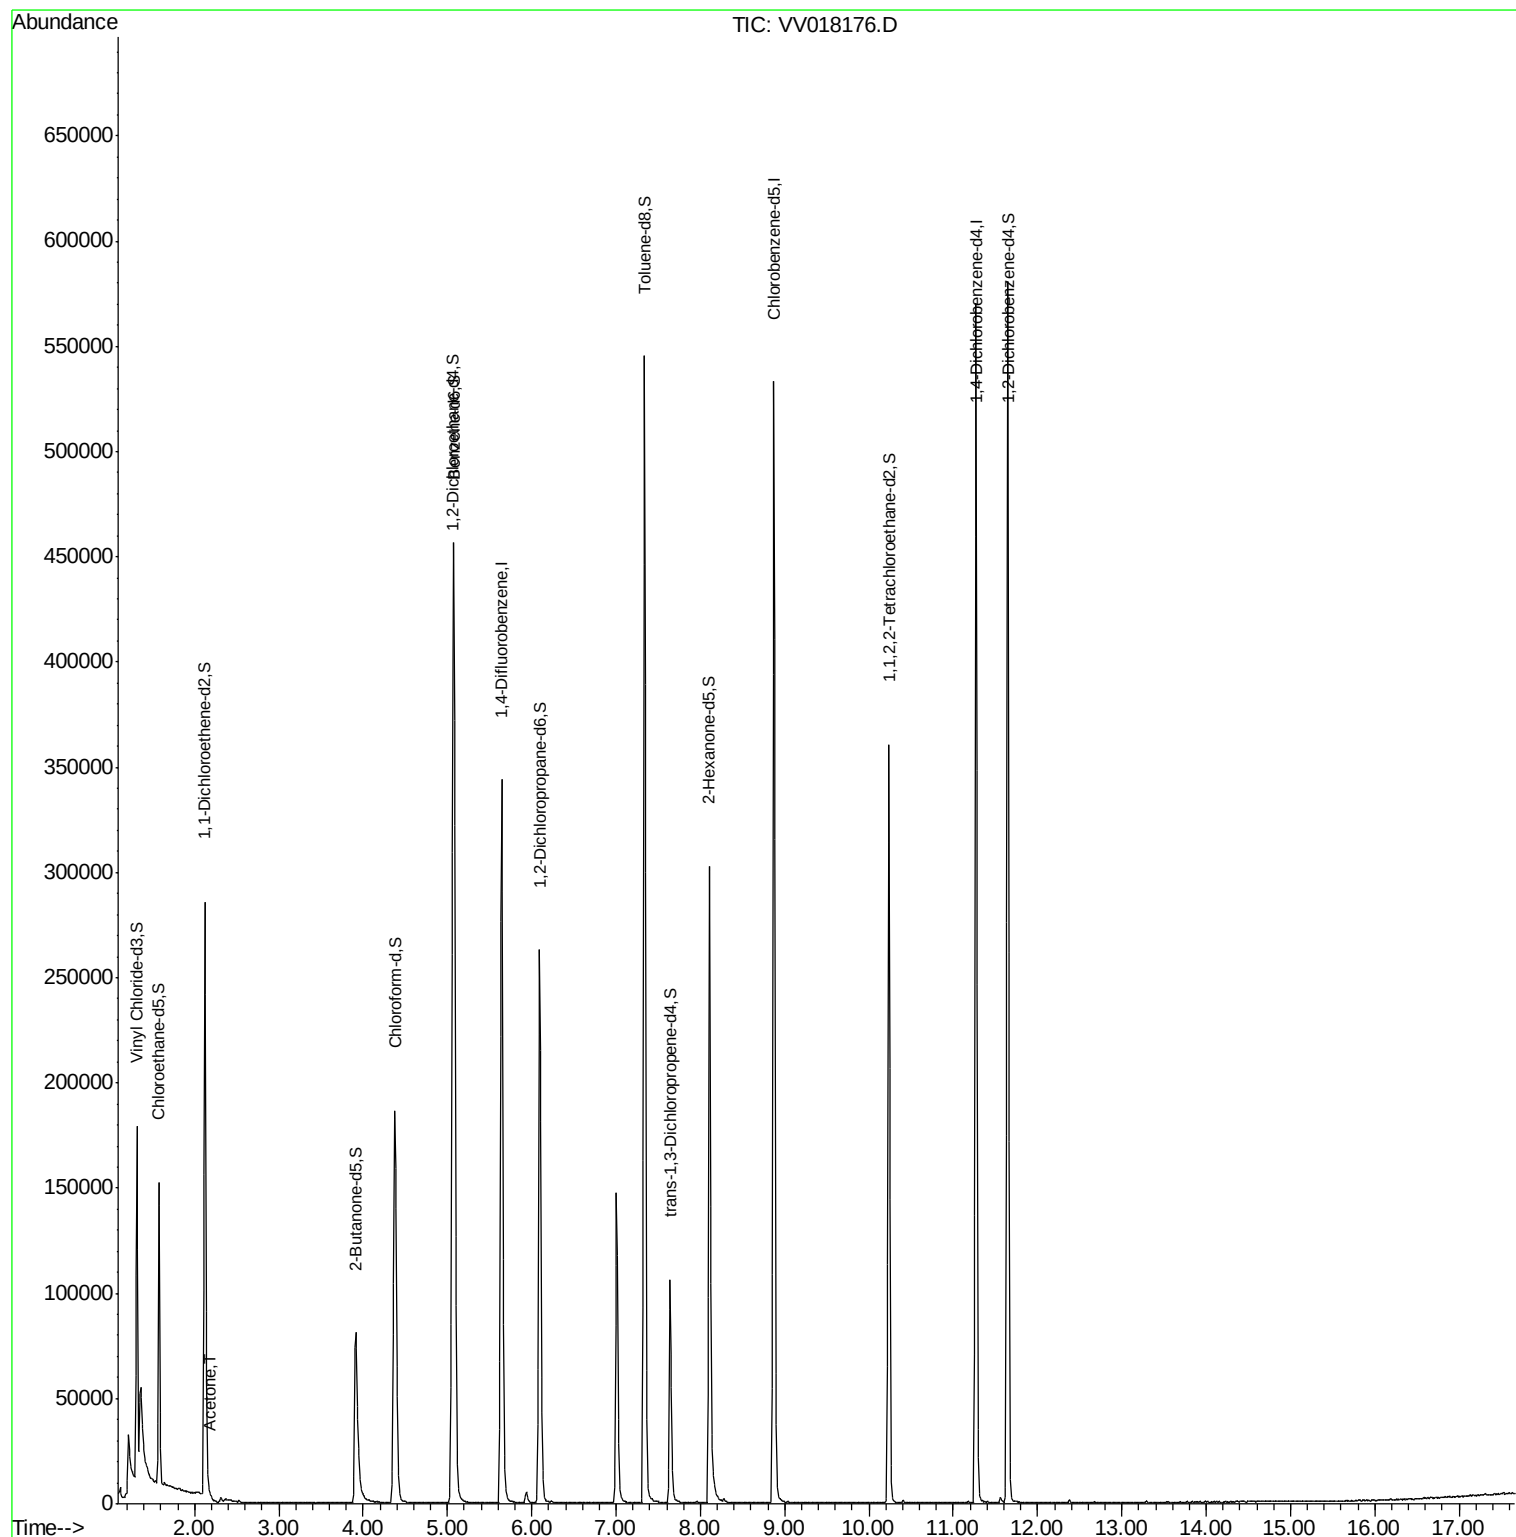

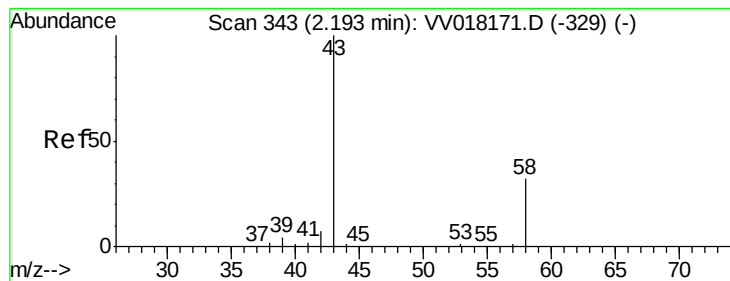

#13

Acetone

Concen: 1.434 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV018176.D

Acq: 10 Sep 2020 13:31

Instrument :
MSVOA_V
ClientSampleId :
BFWQ7

Tot Ion: 43 Resp: 1679

Ion Ratio Lower Upper

43 100

58 25.9 0.0 67.4

