

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091020\
 Data File : VV018178.D
 Acq On : 10 Sep 2020 14:16
 Operator : SY/MD
 Sample : L3957-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWQ9

Quant Time: Sep 11 03:03:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 11 01:30:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	295466	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	294878	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	147017	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	105156	43.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.34%
7) Chloroethane-d5	1.58	69	90583	45.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.94%
11) 1,1-Dichloroethene-d2	2.12	63	151333	34.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.52%
21) 2-Butanone-d5	3.91	46	143370	97.28	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.28%
24) Chloroform-d	4.38	84	194298	46.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.02%
26) 1,2-Dichloroethane-d4	5.06	65	129781	48.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.92%
32) Benzene-d6	5.08	84	396357	46.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.90%
36) 1,2-Dichloropropane-d6	6.09	67	127563	47.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.12%
41) Toluene-d8	7.34	98	354452	46.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.14%
43) trans-1,3-Dichloropropene-	7.64	79	61596	45.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.38%
47) 2-Hexanone-d5	8.11	63	93430	91.96	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.96%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	161999	48.12	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.24%
64) 1,2-Dichlorobenzene-d4	11.65	152	151386	50.14	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.28%


Target Compounds					Ovalue
13) Acetone	2.19	43	3878	3.286 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091020\
Data File : VV018178.D
Acq On : 10 Sep 2020 14:16
Operator : SY/MD
Sample : L3957-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFWQ9

Quant Time: Sep 11 03:03:04 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 11 01:30:09 2020
Response via : Initial Calibration

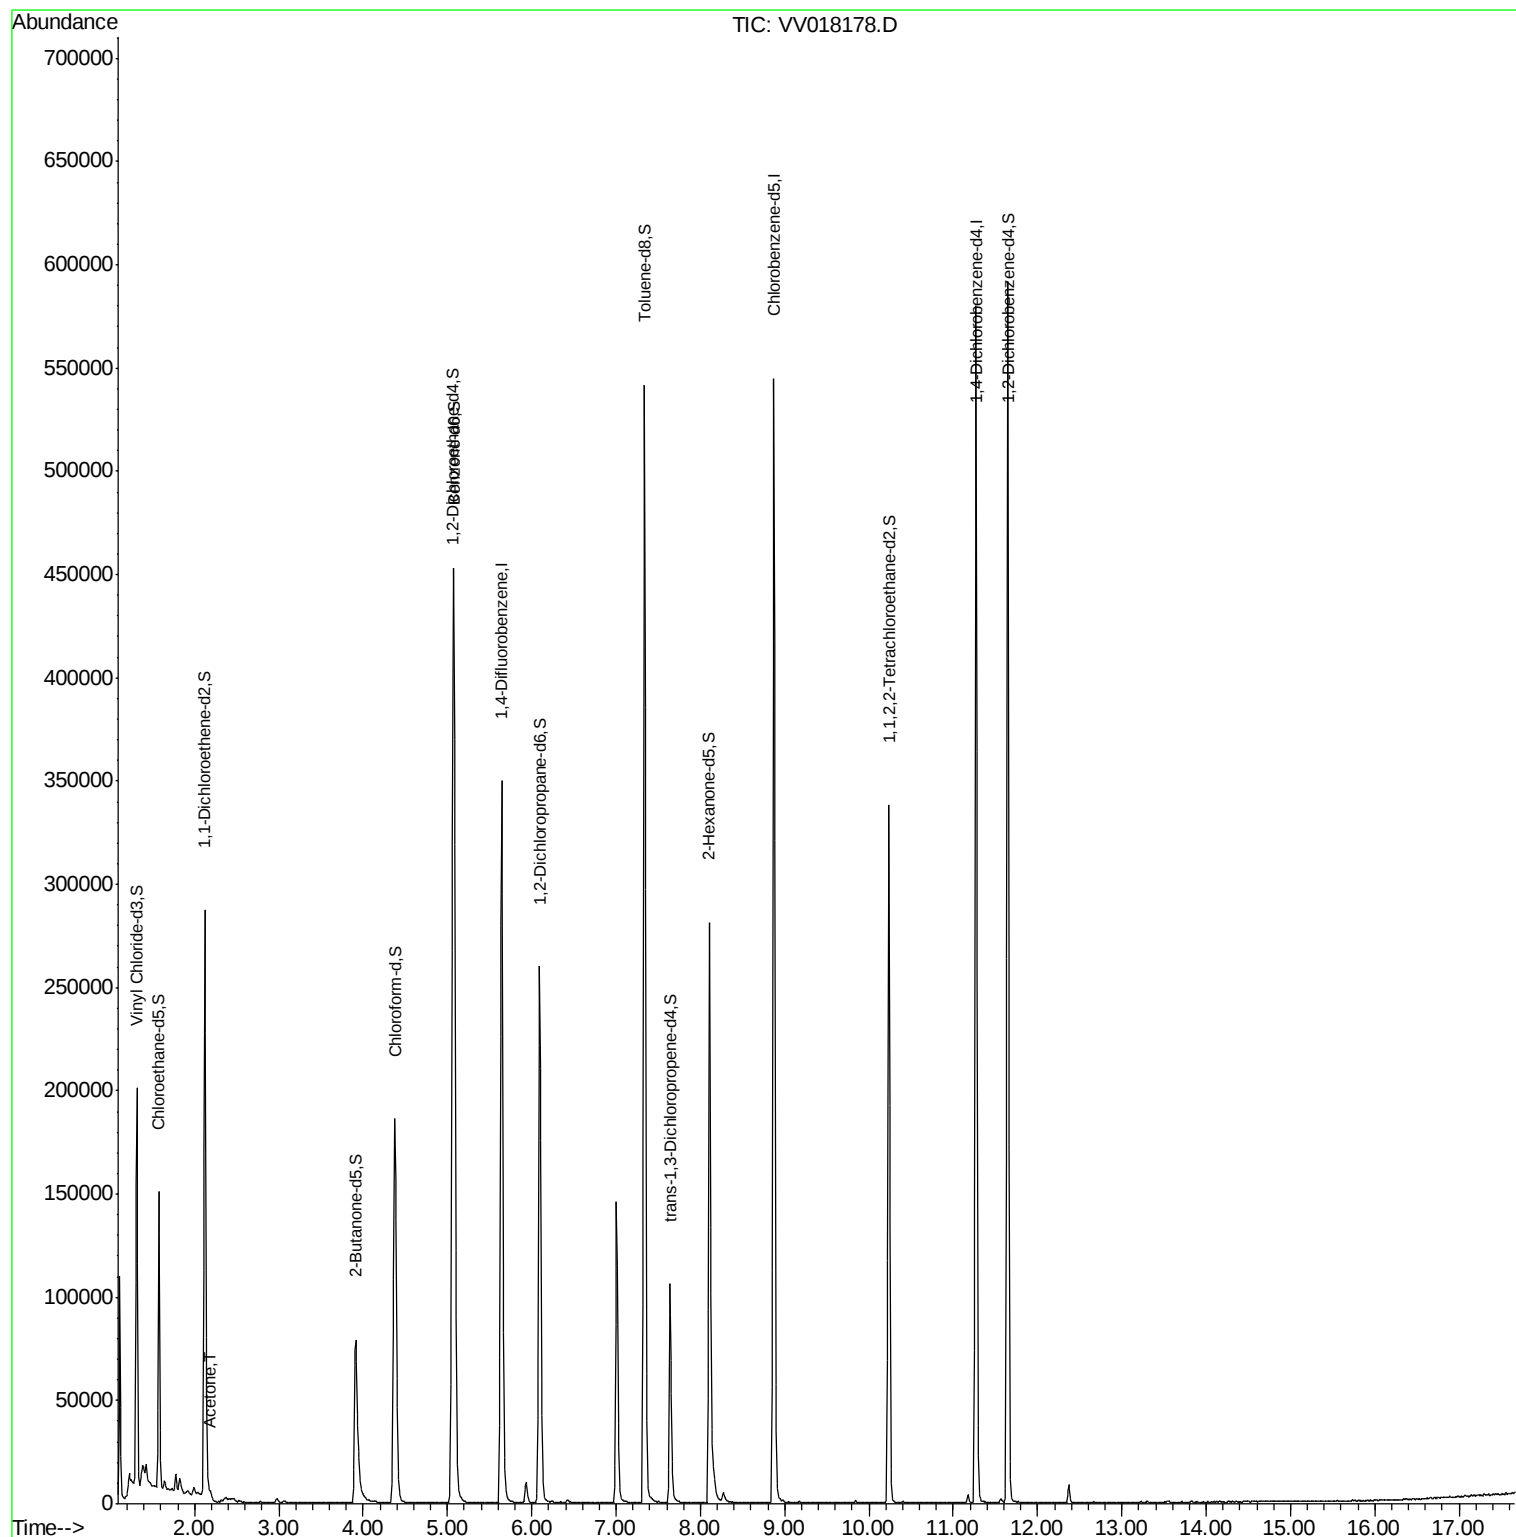

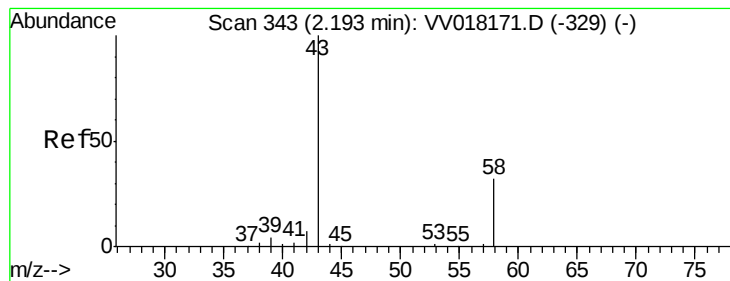

#13
 Acetone
 Concen: 3.286 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. -0.00 min
 Lab File: VV018178.D
 Acq: 10 Sep 2020 14:16

Instrument :
 MSVOA_V
 ClientSampleId :
 BFWQ9

Tot Ion: 43 Resp: 3878
 Ion Ratio Lower Upper
 43 100
 58 30.0 0.0 67.4

