

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091020\
 Data File : VV018182.D
 Acq On : 10 Sep 2020 16:19
 Operator : SY/MD
 Sample : VIBLK60
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK60

Quant Time: Sep 11 03:14:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 11 01:30:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	276156	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	273192	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	135388	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	95102	42.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.52%
7) Chloroethane-d5	1.58	69	83162	45.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.32%
11) 1,1-Dichloroethene-d2	2.12	63	138372	33.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.04%
21) 2-Butanone-d5	3.91	46	131023	95.12	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.12%
24) Chloroform-d	4.38	84	175068	44.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.66%
26) 1,2-Dichloroethane-d4	5.06	65	120079	47.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.94%
32) Benzene-d6	5.08	84	360918	46.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.30%
36) 1,2-Dichloropropane-d6	6.09	67	116964	47.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.14%
41) Toluene-d8	7.34	98	320912	45.02	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.04%
43) trans-1,3-Dichloropropene-	7.64	79	54902	43.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.96%
47) 2-Hexanone-d5	8.11	63	82197	87.33	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.33%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	142941	45.83	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.66%
64) 1,2-Dichlorobenzene-d4	11.65	152	139310	50.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	2672	1.314 ug/L	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091020\
Data File : VV018182.D
Acq On : 10 Sep 2020 16:19
Operator : SY/MD
Sample : VIBLK60
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK60

Quant Time: Sep 11 03:14:38 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 11 01:30:09 2020
Response via : Initial Calibration

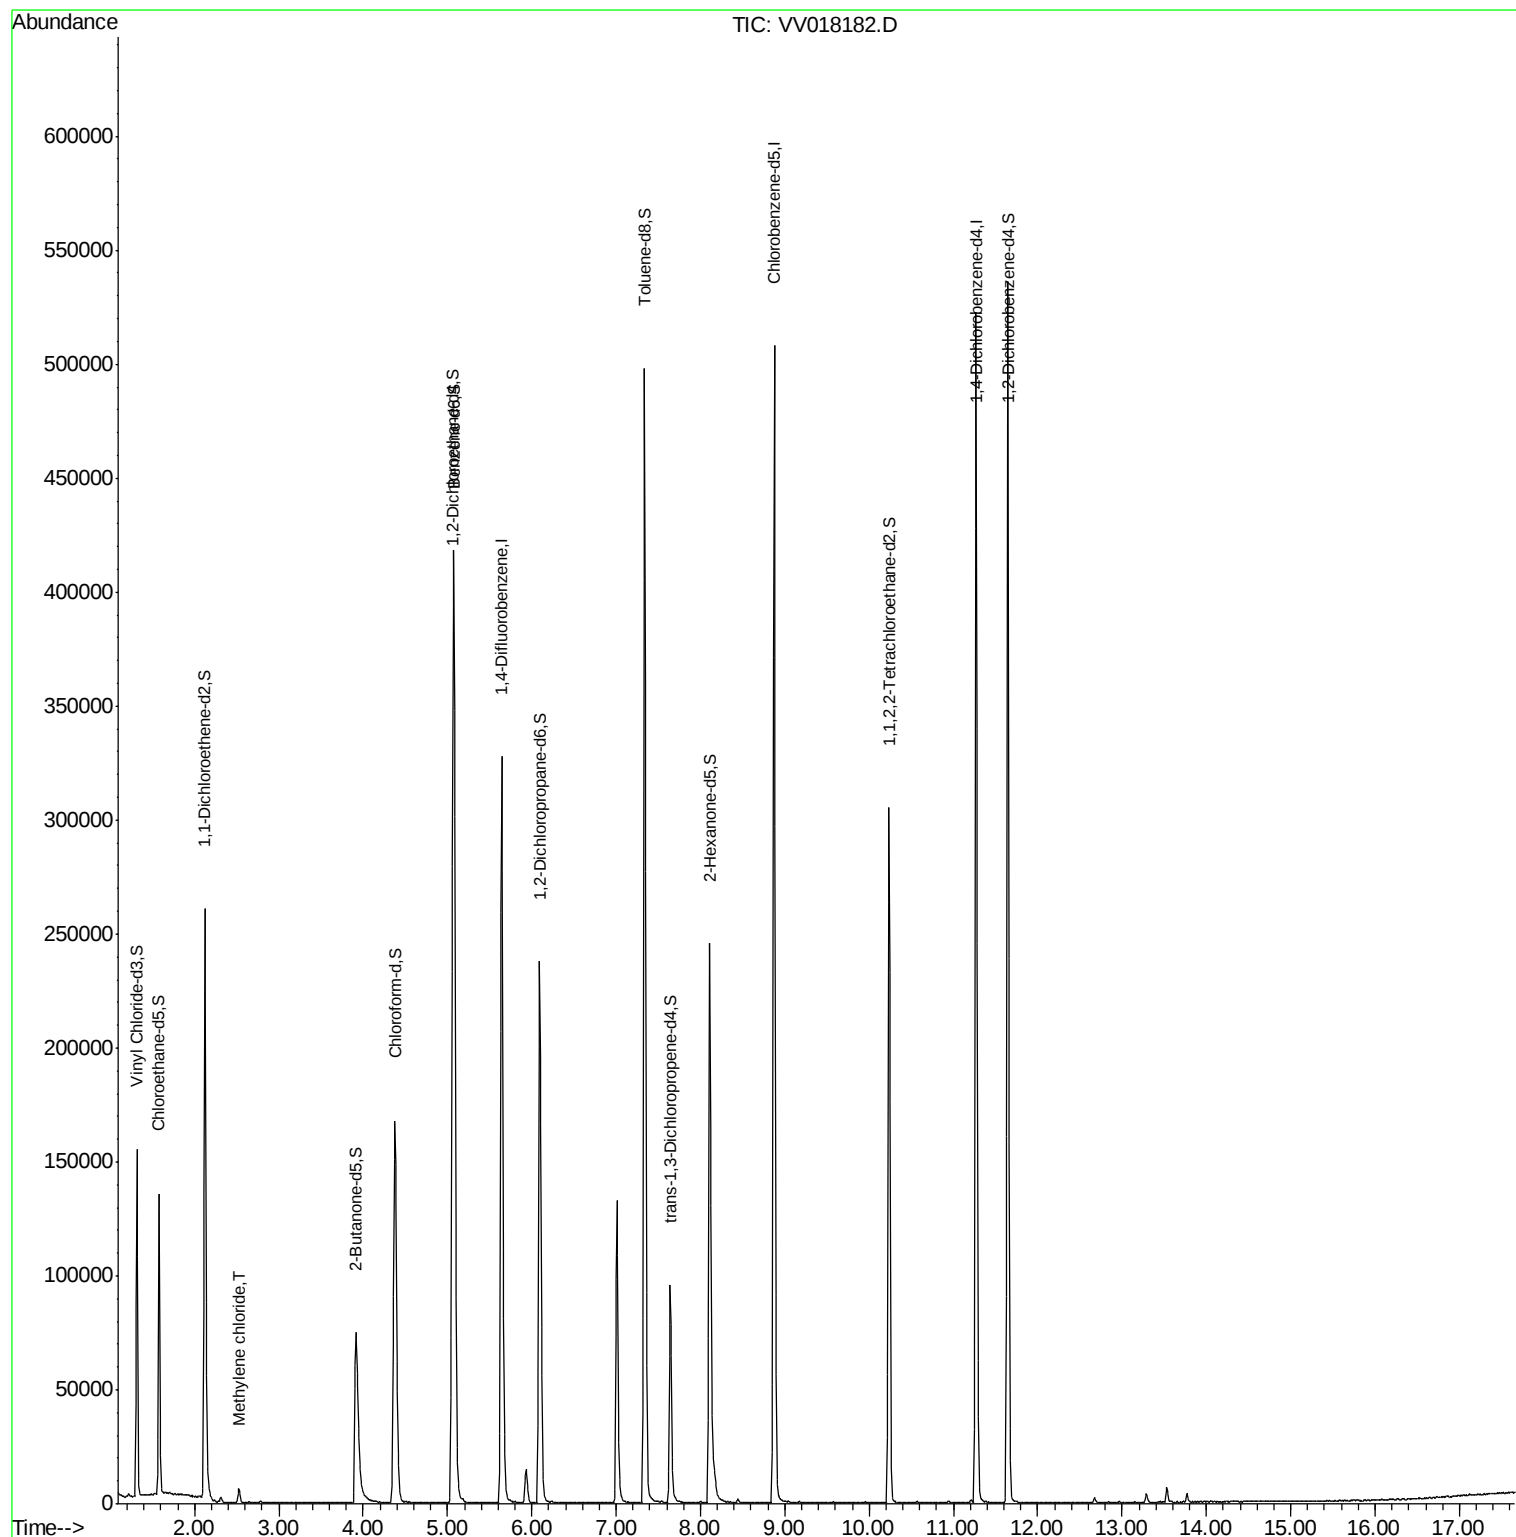

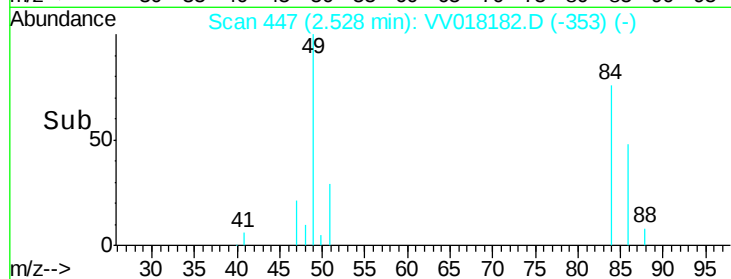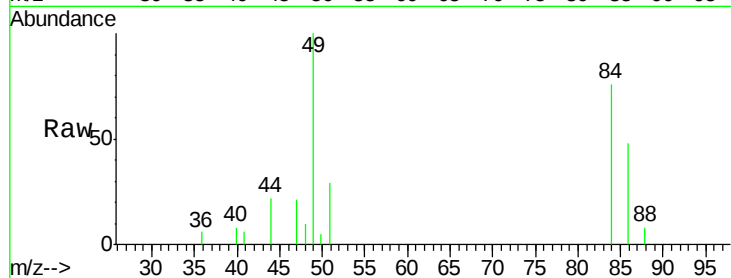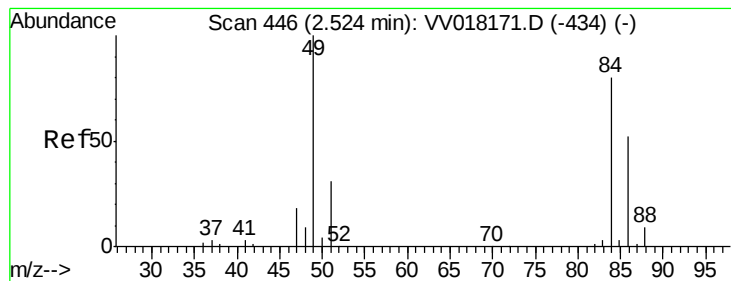

#16
Methvlene chloride
Concen: 1.314 ug/L
RT: 2.53 min Scan# 447
Delta R.T. 0.00 min
Lab File: VV018182.D
Acq: 10 Sep 2020 16:19

Instrument :
MSVOA_V
ClientSampleId :
VIBLK60

Tot Ion: 84 Resp: 2672
Ion Ratio Lower Upper
84 100
86 63.4 44.4 82.4
49 130.9 87.2 162.0

