


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091020\
 Data File : VV018170.D
 Acq On : 10 Sep 2020 09:13
 Operator : SY/MD
 Sample : BFB88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB88

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Fri Sep 11 15:02:16 2020

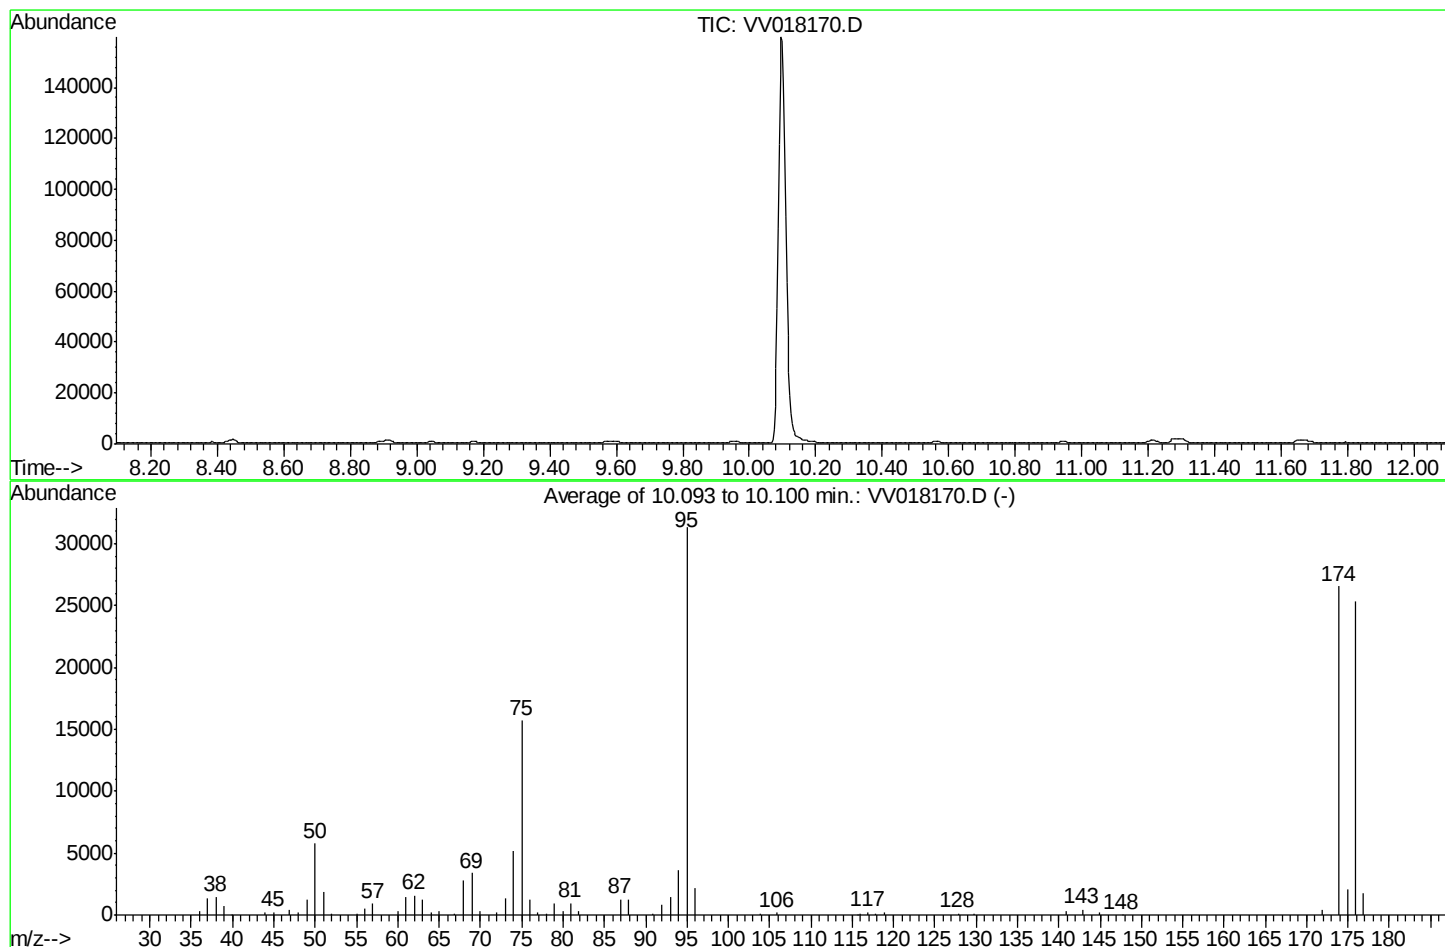

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5781	PASS
75	95	30	80	50.1	15709	PASS
95	95	100	100	100.0	31330	PASS
96	95	5	9	7.0	2183	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	26552	PASS
175	174	5	9	7.7	2045	PASS
176	174	95	101	95.4	25330	PASS
177	176	5	9	6.9	1756	PASS

m/z	Abundance
35.90	283.0
37.00	1353.0
38.00	1478.0
39.00	652.0
40.00	192.0
44.00	484.0
45.00	211.0
46.90	352.0
48.00	244.0
49.00	1161.0
50.00	5598.0
51.00	1732.0
52.00	113.0
55.00	123.0
55.90	481.0
57.00	894.0
59.90	305.0
61.00	1376.0
62.00	1468.0
63.00	1179.0
64.00	219.0
65.10	286.0
68.00	2756.0
69.00	3270.0
70.00	280.0
71.90	150.0
73.00	1308.0
74.00	4884.0
75.00	14800.0
76.00	1237.0
76.90	213.0
78.00	134.0
78.90	980.0
80.00	329.0
80.90	930.0
81.80	236.0
86.90	1190.0
87.90	1155.0
90.80	140.0
92.00	743.0
93.00	1359.0
94.00	3492.0
95.00	29360.0
96.00	2070.0
103.80	137.0
105.90	151.0
116.00	112.0
116.90	235.0
117.80	127.0
118.90	192.0
127.80	126.0
129.70	111.0
140.90	263.0
142.80	424.0
144.90	178.0
147.70	103.0
171.90	364.0
173.90	24408.0
174.90	1881.0
175.90	23568.0
176.90	1674.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
36.00	306.0
37.00	1389.0
38.00	1564.0
39.00	706.0
40.00	191.0
44.00	512.0
44.90	246.0
46.90	385.0
48.00	222.0
49.00	1267.0
50.00	5982.0
51.00	1966.0
52.00	115.0
55.00	122.0
56.00	482.0
57.00	950.0
59.90	296.0
61.00	1542.0
62.00	1626.0
63.00	1311.0
64.00	227.0
65.00	291.0
66.90	105.0
68.00	2873.0
69.00	3558.0
70.00	314.0
71.90	174.0
73.00	1336.0
74.00	5380.0
75.00	16333.0
76.00	1276.0
76.90	220.0
78.00	128.0
78.90	993.0
80.00	366.0
80.90	1003.0
81.80	287.0
86.90	1343.0
87.90	1248.0
90.80	132.0
92.00	812.0
93.00	1486.0
94.00	3801.0
95.00	32440.0
96.00	2250.0
103.80	140.0
105.90	172.0
116.00	139.0
116.90	225.0
117.80	141.0
118.80	210.0
127.80	150.0
129.70	136.0
140.90	303.0
142.90	486.0
144.90	199.0
171.90	395.0
173.90	27456.0
174.90	2123.0
175.90	26208.0
176.90	1805.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
36.00	280.0
37.00	1396.0
38.00	1426.0
39.00	717.0
40.00	168.0
43.90	537.0
44.90	248.0
46.90	380.0
47.90	191.0
49.00	1242.0
50.00	5765.0
51.00	1926.0
52.00	100.0
55.00	117.0
56.00	479.0
57.00	867.0
60.00	282.0
61.00	1545.0
62.00	1649.0
63.00	1299.0
64.00	192.0
64.90	299.0
66.90	102.0
68.00	2839.0
69.00	3396.0
69.90	329.0
71.90	180.0
73.00	1265.0
74.00	5290.0
75.00	15995.0
76.00	1250.0
76.90	216.0
78.00	127.0
78.90	925.0
79.90	346.0
80.90	961.0
81.80	291.0
87.00	1338.0
87.90	1204.0
92.00	861.0
93.00	1483.0
94.00	3692.0
95.00	32192.0
96.00	2230.0
103.80	130.0
105.90	166.0
115.60	114.0
116.00	135.0
116.90	236.0
117.90	125.0
118.80	205.0
127.80	131.0
129.80	134.0
140.90	293.0
142.90	498.0
145.00	187.0
171.90	408.0
173.90	27792.0
174.90	2132.0
175.90	26216.0
176.90	1789.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

Scan 2790 (10.061 min): VV018170.D
BFB88

m/z	Abundance
39.90	161.0
44.00	305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88