

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091021\
 Data File : VV022138.D
 Acq On : 10 Sep 2021 17:14
 Operator : SY/MD
 Sample : VV0910WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Quant Time: Sep 11 01:10:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091021.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 11 01:06:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	9022	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.864	117	8598	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	4195	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	6409	0.493	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	98.000%
4) 1,2-Dichloroethane-d4	5.043	65	3644	0.503	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.069	67	4717	0.515	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.000%
8) Toluene-d8	7.317	98	12603	0.463	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2775	0.492	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	98.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.392	75	5	0.009	ug/L	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091021\
Data File : VV022138.D
Acq On : 10 Sep 2021 17:14
Operator : SY/MD
Sample : VV0910WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK204


Quant Time: Sep 11 01:10:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091021.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 11 01:06:11 2021
Response via : Initial Calibration

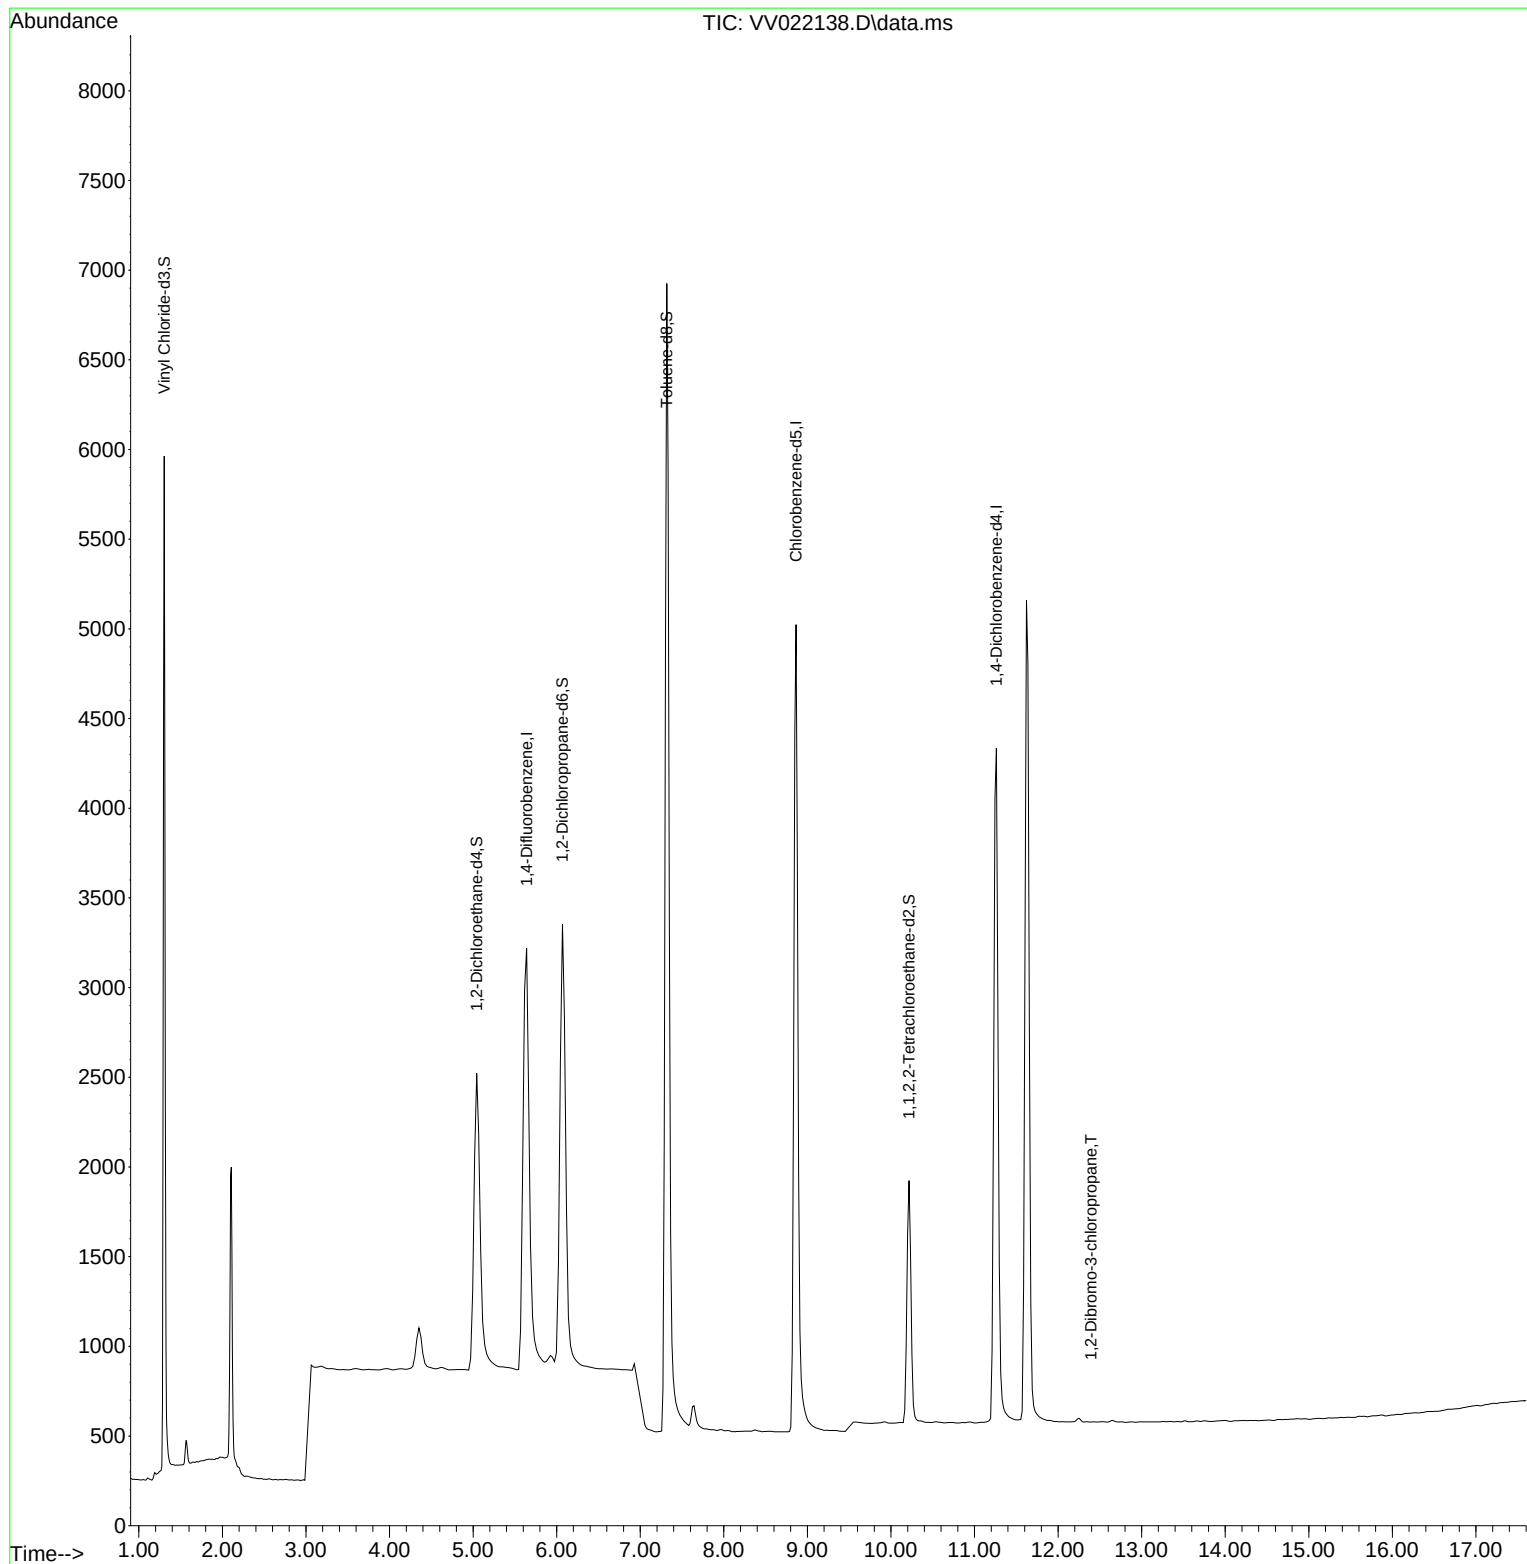

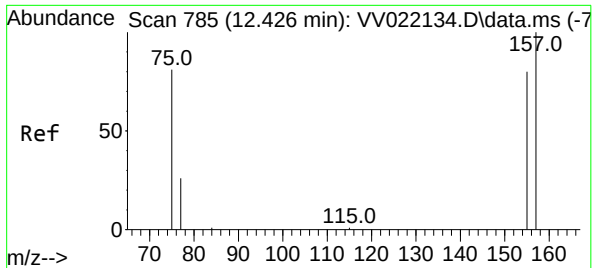

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.009 ug/L
 RT: 12.392 min Scan# 783
 Delta R.T. -0.034 min
 Lab File: VV022138.D
 Acq: 10 Sep 2021 17:14

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

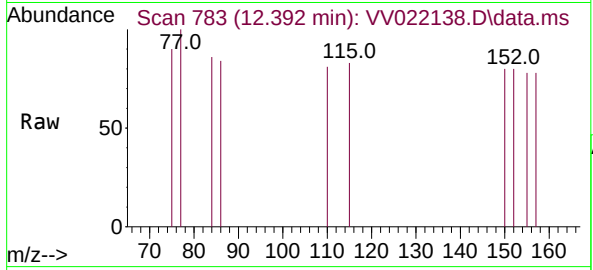

Tgt Ion: 75 Resp: 5

Ion	Ratio	Lower	Upper
75	100		
157	87.1	88.5	132.7#
155	87.1	76.0	114.0

