

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091119\
 Data File : VV012673.D
 Acq On : 11 Sep 2019 15:19
 Operator : SY/MD
 Sample : K4809-01
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFDB8

Quant Time: Sep 12 07:56:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 12 07:16:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	411640	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	411765	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	165098	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	165596	5.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.60%
7) Chloroethane-d5	1.58	69	137543	5.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.20%
11) 1,1-Dichloroethene-d2	2.13	63	205862	4.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.40%
20) 2-Butanone-d5	3.93	46	357356	53.18	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.36%
24) Chloroform-d	4.40	84	279145	5.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.00%
26) 1,2-Dichloroethane-d4	5.08	65	138324	5.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.00%
32) Benzene-d6	5.10	84	558526	5.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.60%
36) 1,2-Dichloropropane-d6	6.12	67	175394	5.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.20%
41) Toluene-d8	7.36	98	448382	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
43) trans-1,3-Dichloropropene-	7.66	79	51581	4.80	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.00%
46) 2-Hexanone-d5	8.13	63	165287	40.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.30%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	99799	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	161860	5.73	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.60%


Target Compounds				Ovalue
13) Acetone	2.19	43	21803	5.536 ug/L 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091119\
Data File : VV012673.D
Acq On : 11 Sep 2019 15:19
Operator : SY/MD
Sample : K4809-01
Misc : 25mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFDB8

Quant Time: Sep 12 07:56:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 12 07:16:59 2019
Response via : Initial Calibration

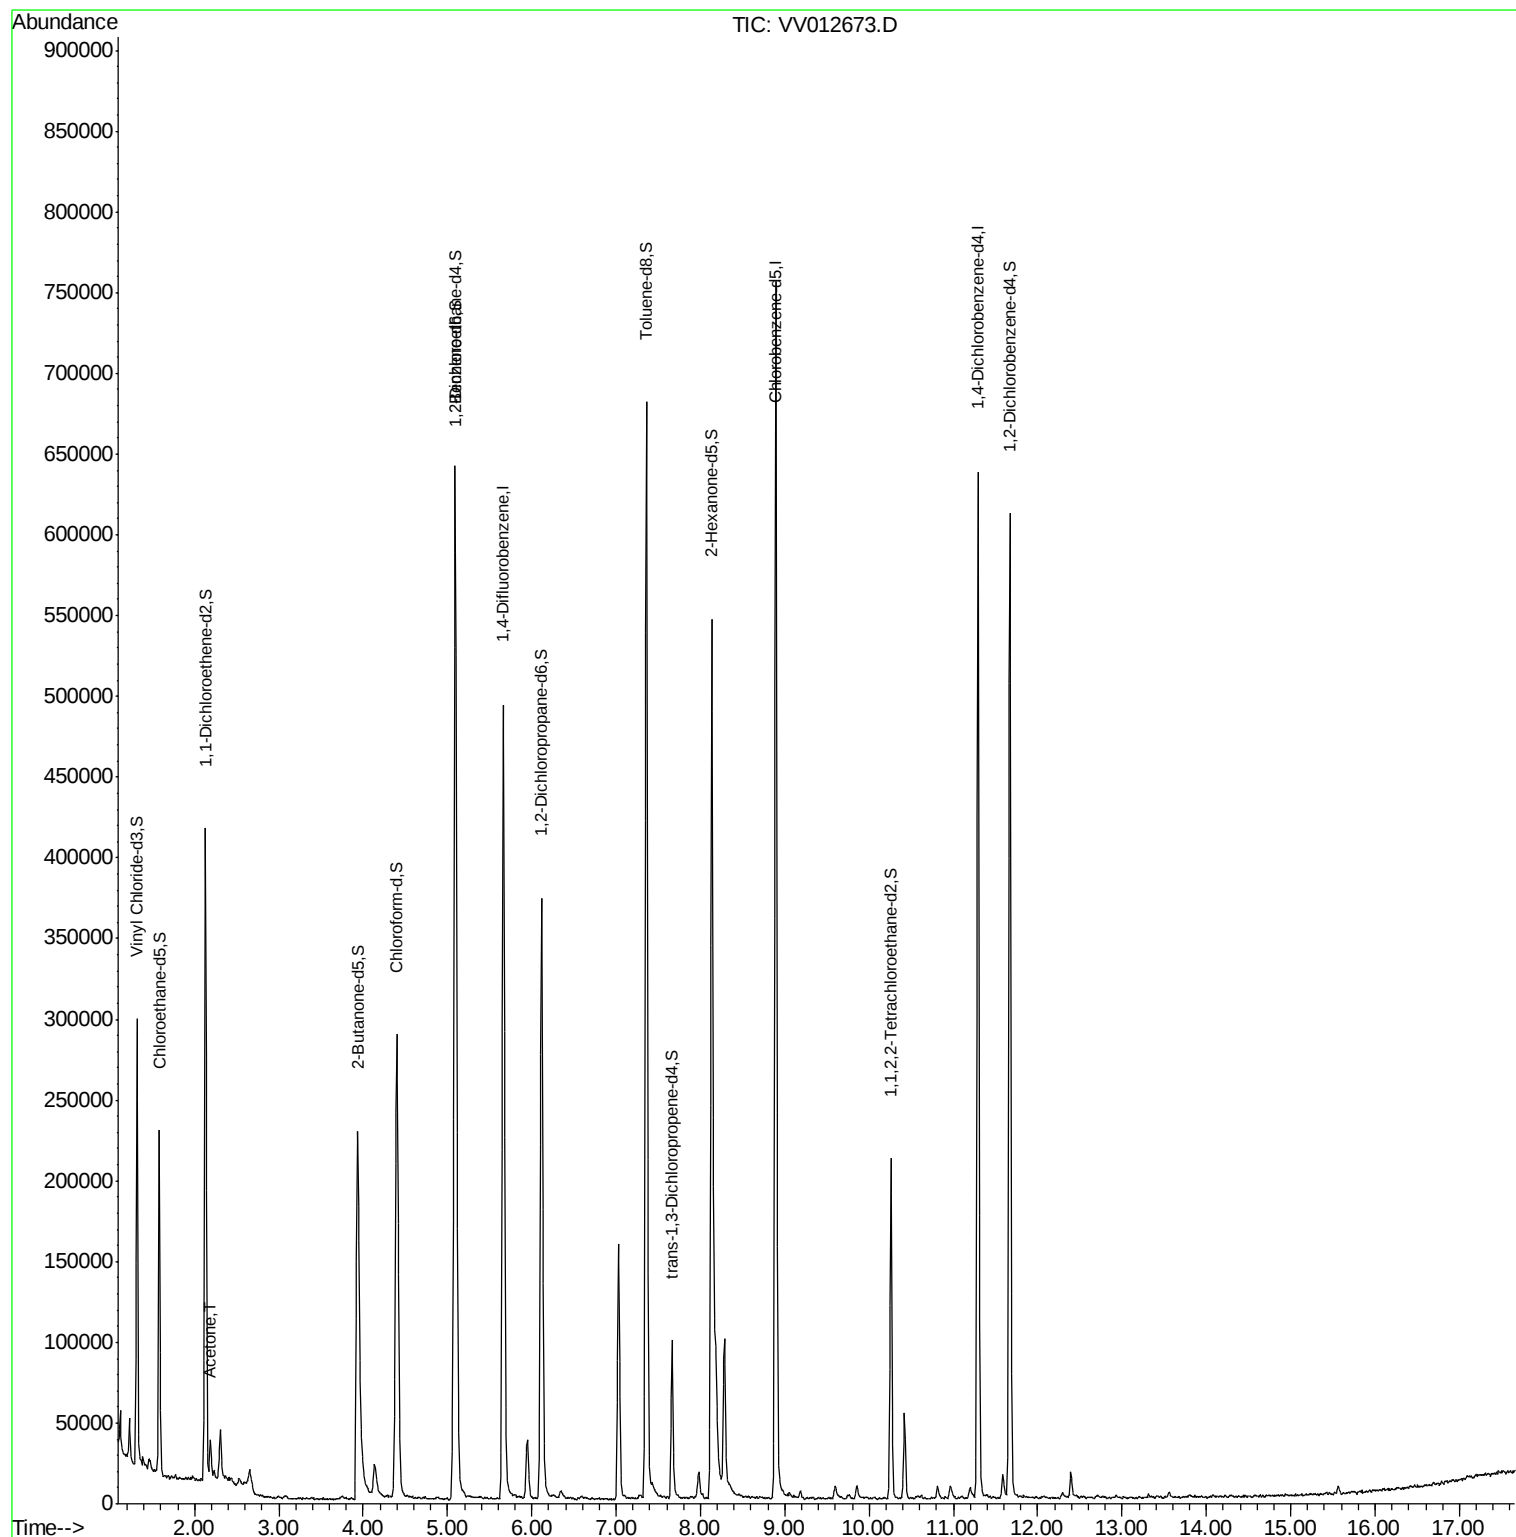

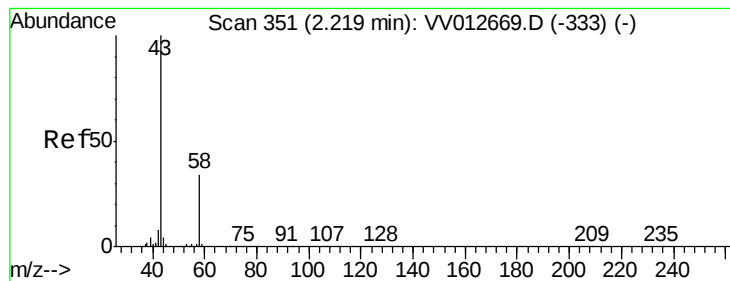

#13

Acetone

Concen: 5.536 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.03 min

Lab File: VV012673.D

Acq: 11 Sep 2019 15:19


Instrument :
MSVOA_V
ClientSampleId :
BFDB8

Tot Ion: 43 Resp: 21803

Ion Ratio Lower Upper

43 100

58 34.8 0.0 67.4

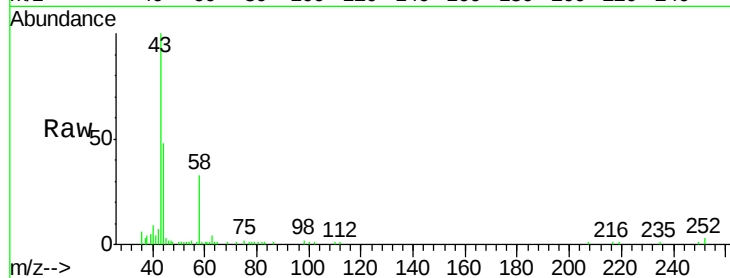

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

