

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091119\
 Data File : VV012674.D
 Acq On : 11 Sep 2019 15:45
 Operator : SY/MD
 Sample : K4809-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFDB9

Quant Time: Sep 12 08:13:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 12 07:16:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	395369	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	400796	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	159566	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	162677	6.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	121.40%
7) Chloroethane-d5	1.58	69	132802	5.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.80%
11) 1,1-Dichloroethene-d2	2.13	63	201896	4.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.20%
20) 2-Butanone-d5	3.96	46	401318	62.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.36%
24) Chloroform-d	4.40	84	278753	5.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.40%
26) 1,2-Dichloroethane-d4	5.08	65	141240	6.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.00%
32) Benzene-d6	5.10	84	554603	5.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.80%
36) 1,2-Dichloropropane-d6	6.12	67	174984	5.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.00%
41) Toluene-d8	7.36	98	444622	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
43) trans-1,3-Dichloropropene-	7.66	79	54088	5.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.40%
46) 2-Hexanone-d5	8.14	63	186435	47.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.20%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	111579	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	166527	6.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.00%#


Target Compounds				Ovalue
13) Acetone	2.21	43	22909	6.056 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091119\
Data File : VV012674.D
Acq On : 11 Sep 2019 15:45
Operator : SY/MD
Sample : K4809-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFDB9

Quant Time: Sep 12 08:13:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 12 07:16:59 2019
Response via : Initial Calibration

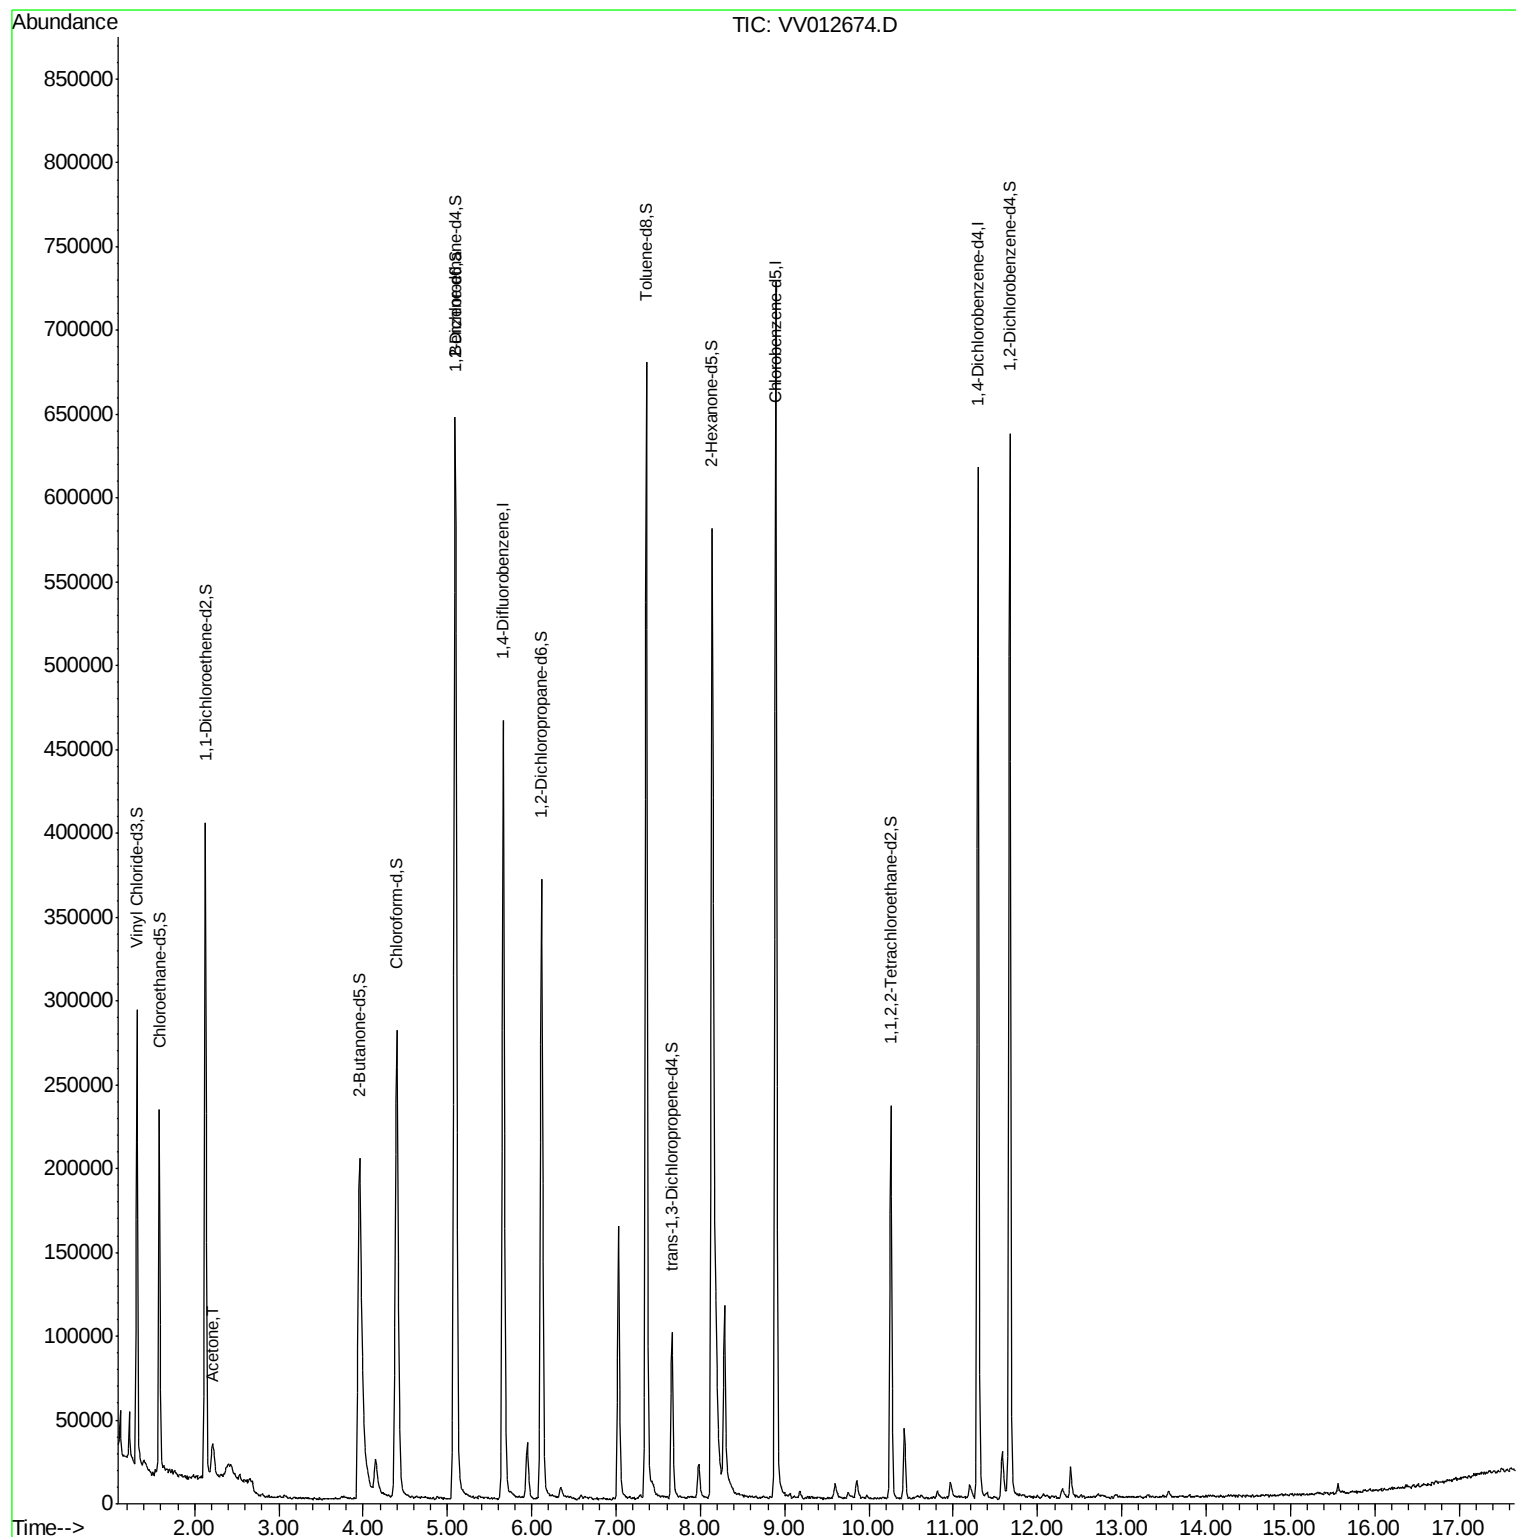

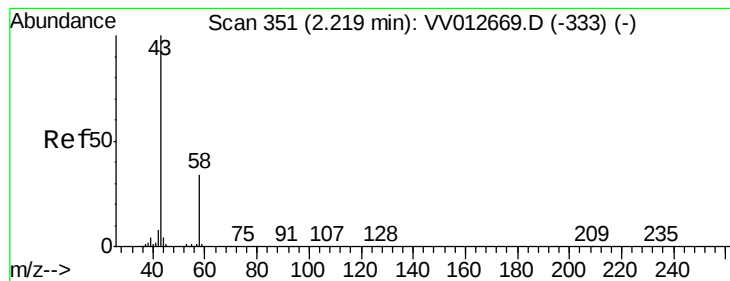

#13

Acetone

Concen: 6.056 ug/L

RT: 2.21 min Scan# 349

Delta R.T. -0.01 min

Lab File: VV012674.D

Acq: 11 Sep 2019 15:45


Instrument :
MSVOA_V
ClientSampleId :
BFDB9

Tot Ion: 43 Resp: 22909

Ion Ratio Lower Upper

43 100

58 34.4 0.0 67.4

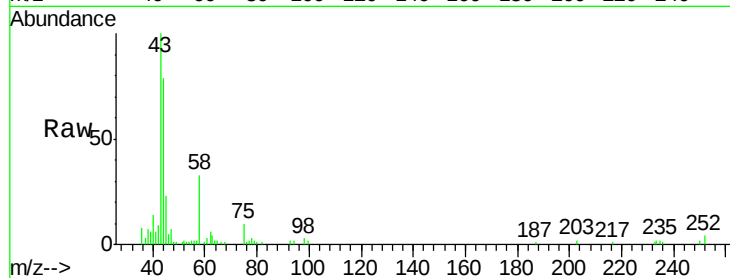

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

2.21

10000

8000

6000

4000

2000

0

Time--> 2.10 2.15 2.20 2.25 2.30

