


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV091119\
Data File : VV012668.D
Acq On : 11 Sep 2019 08:48
Operator : SY/MD
Sample : BFB35
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 12 12:15:43 2019

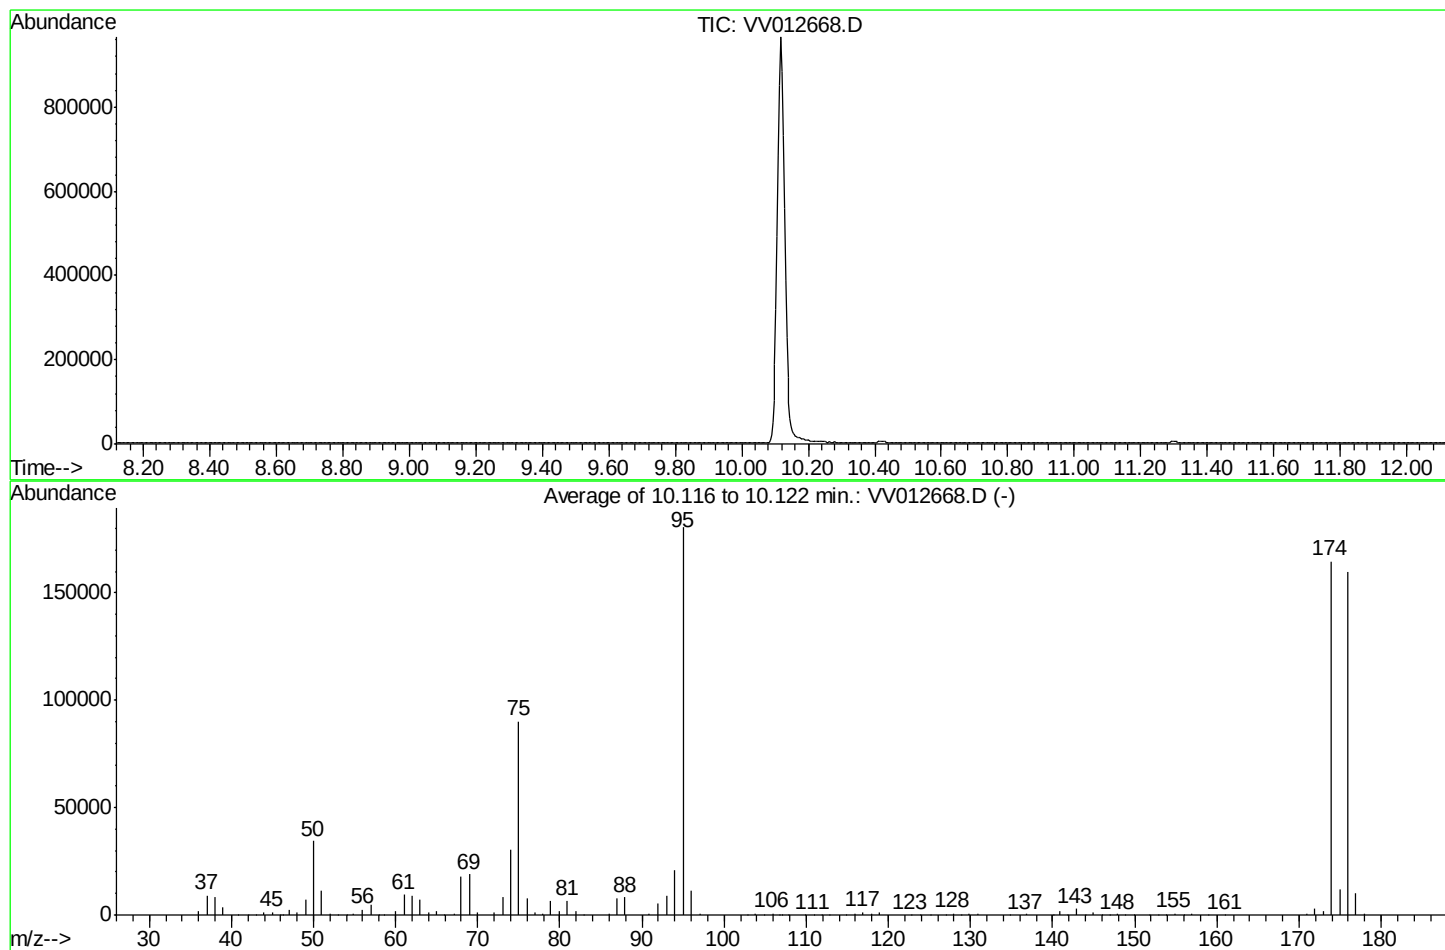

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	34490	PASS
75	95	30	80	49.9	90037	PASS
95	95	100	100	100.0	180522	PASS
96	95	5	9	6.4	11556	PASS
173	174	0.00	2	1.2	2021	PASS
174	95	50	120	91.3	164821	PASS
175	174	5	9	7.1	11745	PASS
176	174	95	101	97.0	159808	PASS
177	176	5	9	6.4	10277	PASS

m/z	Abundance
36.00	1863.0
37.00	9617.0
38.00	8376.0
39.00	3871.0
40.00	1365.0
42.00	112.0
43.10	146.0
44.00	1920.0
45.00	1586.0
45.90	268.0
46.20	308.0
47.00	2513.0
47.90	1440.0
49.00	7177.0
50.00	36056.0
51.00	11797.0
51.90	485.0
52.90	259.0
54.10	169.0
54.90	530.0
56.00	2549.0
57.00	5139.0
57.90	164.0
58.60	109.0
60.00	1830.0
61.00	9715.0
62.00	9580.0
63.00	7927.0
64.00	1458.0
65.00	1900.0
66.00	269.0
67.10	439.0
68.00	18864.0
69.00	19984.0
70.00	1607.0
71.90	1192.0
73.00	8408.0
74.00	31072.0
75.00	93528.0
76.00	7853.0
77.00	1197.0
78.00	851.0
78.90	6616.0
80.00	1741.0
80.90	7017.0
81.90	1672.0
82.90	162.0
86.00	456.0
87.00	8126.0
88.00	8380.0
90.80	549.0
92.00	5248.0
93.00	9017.0
94.00	22080.0
95.00	184960.0
96.00	11927.0
97.00	340.0
102.90	113.0
103.80	755.0
104.90	316.0
105.90	722.0
106.70	150.0
107.10	151.0
107.90	113.0
110.90	181.0
111.90	116.0
112.80	170.0
114.90	208.0
115.90	654.0
116.90	1281.0
117.90	651.0
118.90	1189.0
122.80	129.0
124.00	116.0
127.00	106.0
127.90	774.0
128.90	314.0
129.80	752.0
130.90	323.0
134.80	227.0
136.80	318.0
140.10	225.0
140.90	1719.0
141.80	323.0
142.90	2923.0
144.00	250.0
144.90	1029.0
146.00	300.0
146.90	123.0
147.90	374.0
148.80	130.0
149.90	317.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

151.80	122.0
152.80	204.0
153.80	106.0
154.90	707.0
156.00	109.0
156.80	416.0
158.90	365.0
161.00	161.0
171.00	417.0
171.90	2879.0
173.00	2076.0
173.90	165248.0
174.90	12085.0
175.90	159424.0
176.90	10268.0
178.00	347.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	1803.0
37.00	9675.0
38.00	8448.0
39.00	3622.0
40.00	1350.0
42.00	122.0
43.00	193.0
44.00	1880.0
45.00	1617.0
45.90	181.0
46.30	262.0
47.00	2387.0
47.90	1404.0
49.00	7101.0
50.00	35544.0
51.00	12000.0
52.00	449.0
52.90	258.0
54.10	172.0
54.90	519.0
56.00	2763.0
57.00	5207.0
57.90	246.0
60.00	1731.0
61.00	9923.0
62.00	9253.0
63.00	7650.0
64.00	1355.0
65.00	1904.0
65.90	304.0
67.10	428.0
68.00	18640.0
69.00	19624.0
70.00	1611.0
72.00	951.0
73.00	8372.0
74.00	31224.0
75.00	92664.0
76.00	7742.0
77.00	1163.0
78.00	890.0
78.90	6580.0
80.00	1727.0
80.90	6836.0
81.90	1631.0
82.90	146.0
86.00	402.0
86.90	8147.0
87.90	8662.0
90.80	559.0
92.00	5275.0
93.00	9016.0
94.00	21224.0
95.00	185920.0
96.00	11904.0
97.00	453.0
102.90	126.0
103.80	718.0
104.80	343.0
106.00	791.0
107.00	173.0
107.90	128.0
109.90	130.0
110.90	232.0
112.00	110.0
112.90	131.0
114.90	206.0
116.00	730.0
116.90	1389.0
117.90	723.0
118.90	1260.0
122.80	132.0
123.90	127.0
125.10	123.0
127.00	146.0
127.90	759.0
128.90	312.0
129.80	650.0
130.90	376.0
134.80	261.0
136.80	356.0
140.10	238.0
140.90	1785.0
141.80	261.0
142.90	2846.0
144.10	244.0
144.90	1022.0
146.00	241.0
146.90	124.0
147.90	397.0
148.80	132.0
149.90	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

151.80	101.0
152.80	172.0
153.70	125.0
154.90	680.0
156.00	125.0
156.80	398.0
158.90	280.0
161.00	206.0
170.90	501.0
171.90	3030.0
173.00	2064.0
173.90	170624.0
175.00	12013.0
175.90	166208.0
176.90	10682.0
177.90	375.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	1558.0
37.00	8441.0
38.00	7661.0
39.00	3194.0
40.00	1340.0
40.80	105.0
42.00	130.0
43.00	216.0
43.90	1820.0
45.00	1475.0
46.20	255.0
47.00	2010.0
48.00	1165.0
49.00	6599.0
50.00	31872.0
51.00	10604.0
52.00	416.0
52.90	278.0
54.10	155.0
54.90	460.0
56.00	2598.0
57.00	4592.0
58.00	302.0
60.00	1558.0
61.00	8908.0
62.00	8431.0
63.00	6671.0
64.00	1181.0
65.00	1671.0
65.90	366.0
67.10	420.0
68.00	16704.0
69.00	17208.0
70.00	1285.0
72.00	773.0
73.00	7546.0
74.00	28304.0
75.00	83920.0
76.00	7056.0
77.00	1042.0
77.90	843.0
78.90	5973.0
79.90	1569.0
80.90	6054.0
81.90	1415.0
82.90	138.0
86.00	285.0
86.90	7196.0
87.90	7717.0
90.80	613.0
92.00	4873.0
93.00	8036.0
94.00	18712.0
95.00	170688.0
96.00	10837.0
97.00	436.0
102.80	128.0
103.80	607.0
104.80	293.0
106.00	739.0
107.00	190.0
107.90	128.0
109.90	154.0
110.90	253.0
111.90	112.0
112.90	137.0
114.80	203.0
115.90	781.0
116.90	1396.0
117.90	765.0
118.90	1253.0
122.70	112.0
123.80	129.0
125.10	124.0
127.10	142.0
127.90	611.0
128.90	263.0
129.90	599.0
130.90	367.0
134.80	270.0
136.80	317.0
140.10	225.0
140.90	1617.0
141.90	193.0
142.90	2488.0
144.10	204.0
144.90	1035.0
145.90	228.0
147.90	391.0
148.80	110.0
149.80	161.0
152.80	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

153.70	111.0
154.90	606.0
156.00	119.0
156.90	366.0
159.00	158.0
161.00	200.0
170.90	549.0
171.90	2951.0
172.90	1925.0
173.90	158592.0
175.00	11138.0
175.90	153792.0
176.90	9882.0
177.90	338.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

Scan 2794 (10.074 min): VV012668.D
BFB35

m/z	Abundance
39.90	1455.0
41.10	112.0
43.90	929.0
44.80	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35