

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032033.D
 Acq On : 11 Sep 2023 17:56
 Operator : SY/MD
 Sample : 04306-13 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4K9

Quant Time: Sep 12 06:01:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 09 21:51:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	113608	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	117009	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	61251	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	18161	4.733	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.600%
7) Chloroethane-d5	1.532	69	22958	5.223	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.400%
11) 1,1-Dichloroethene-d2	2.060	65	10354	4.585	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	91.600%
20) 2-Butanone-d5	3.815	46	98458	53.008	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.020%
24) Chloroform-d	4.256	84	56918	4.383	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	4.950	65	29858	4.462	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.200%
32) Benzene-d6	4.966	84	110209	4.139	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
36) 1,2-Dichloropropane-d6	5.995	67	38275	4.077	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.600%
41) Toluene-d8	7.249	98	96283	3.897	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	7.564	79	10488	3.063	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.200%
46) 2-Hexanone-d5	8.034	63	77909	42.680	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.360%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	29174	4.331	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.600%
66) 1,2-Dichlorobenzene-d4	11.567	152	37475	3.778	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	75.600%#
Target Compounds						
					Qvalue	
16) Methylene chloride	2.452	84	2344	0.282	ug/L	73
17) Methyl tert-butyl Ether	2.716	73	3345	0.211	ug/L	# 87
22) cis-1,2-Dichloroethene	3.828	96	4553	0.682	ug/L	95
34) Trichloroethene	5.838	95	64342	8.168	ug/L	98
65) 1,4-Dichlorobenzene	11.214	146	1828	0.118	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032033.D
Acq On : 11 Sep 2023 17:56
Operator : SY/MD
Sample : 04306-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K9

Quant Time: Sep 12 06:01:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 09 21:51:31 2023
Response via : Initial Calibration

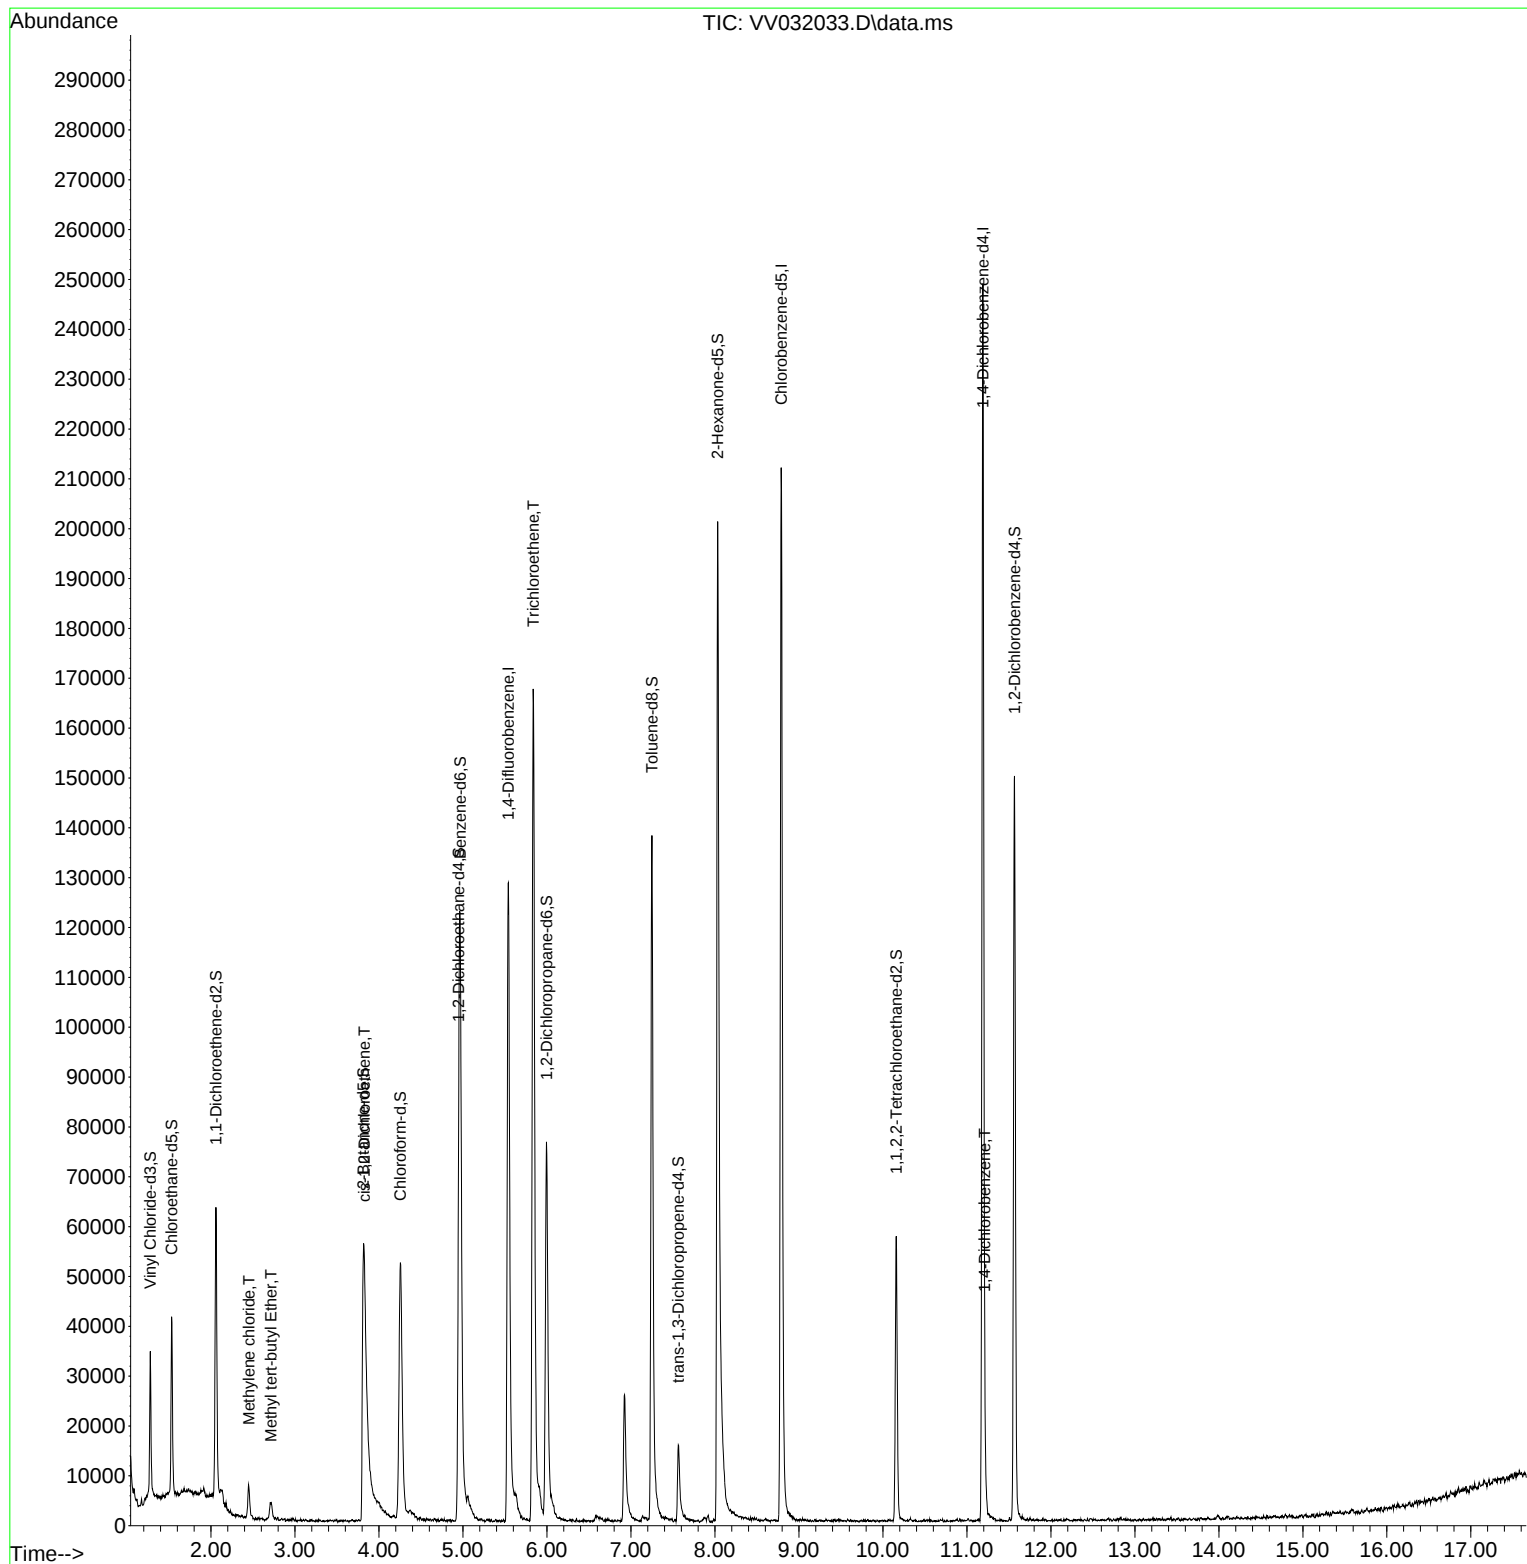




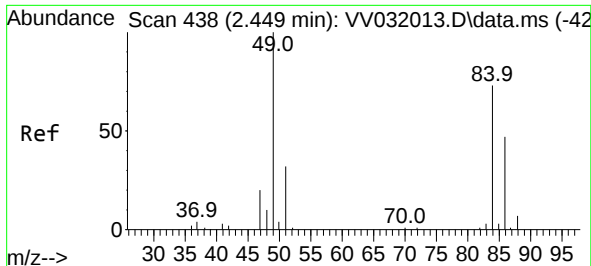


#16
Methylene chloride
Concen: 0.282 ug/L
RT: 2.452 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV032033.D
Acq: 11 Sep 2023 17:56

Instrument :
MSVOA_V
ClientSampleId :
BH4K9

Tgt Ion: 84 Resp: 2344




Ion	Ratio	Lower	Upper
84	100		
86	78.5	42.6	79.2
49	159.6	88.5	164.4

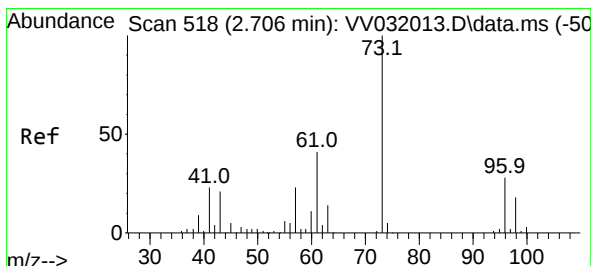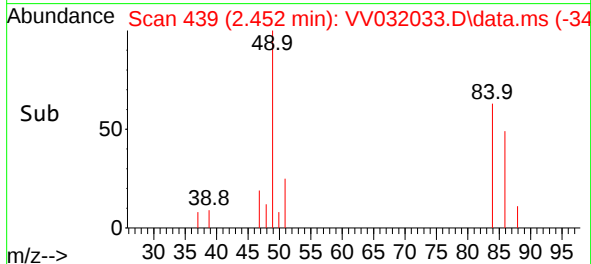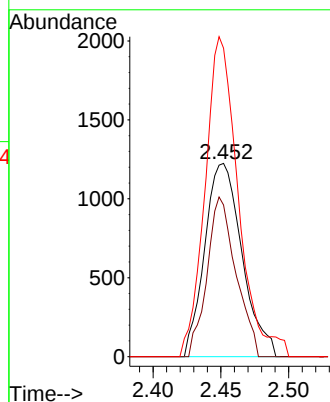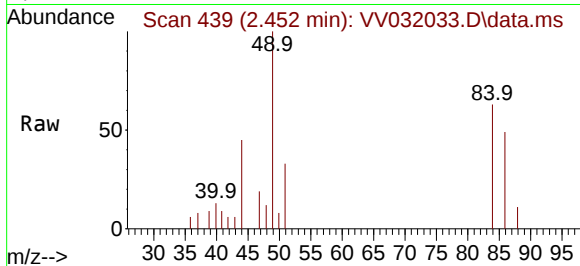


#17
Methyl tert-butyl Ether
Concen: 0.211 ug/L
RT: 2.716 min Scan# 521
Delta R.T. 0.010 min
Lab File: VV032033.D
Acq: 11 Sep 2023 17:56

Tgt Ion: 73 Resp: 3345

Ion	Ratio	Lower	Upper
73	100		
43	28.3	15.6	23.4#
57	26.2	17.8	26.8


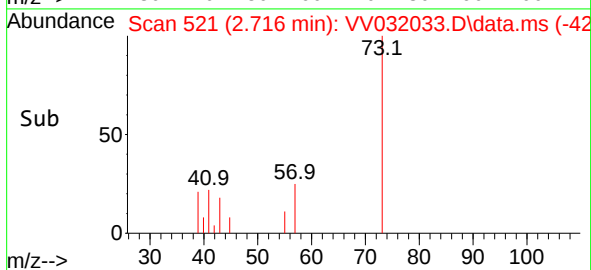
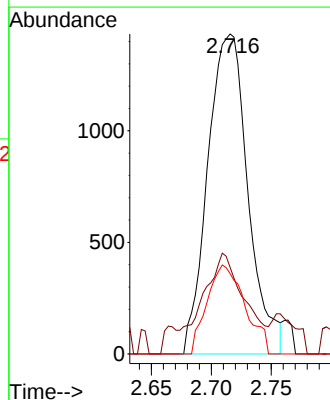
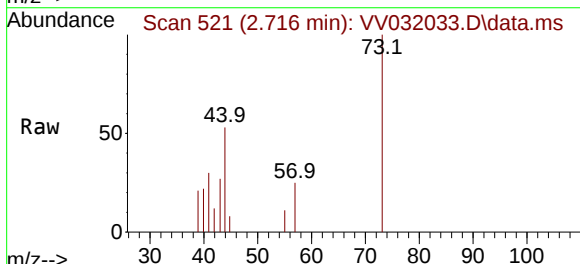


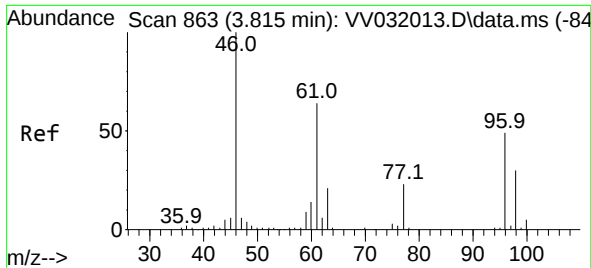

#22
cis-1,2-Dichloroethene
Concen: 0.682 ug/L
RT: 3.828 min Scan# 867
Delta R.T. 0.013 min
Lab File: VV032033.D
Acq: 11 Sep 2023 17:56




Instrument :
MSVOA_V
ClientSampleId :
BH4K9


Tgt Ion: 96 Resp: 4553
Ion Ratio Lower Upper
96 100
61 142.4 94.1 174.8
98 62.6 43.8 81.4

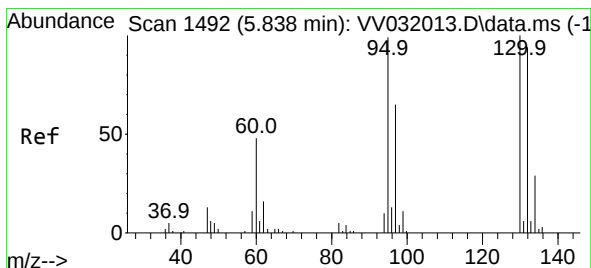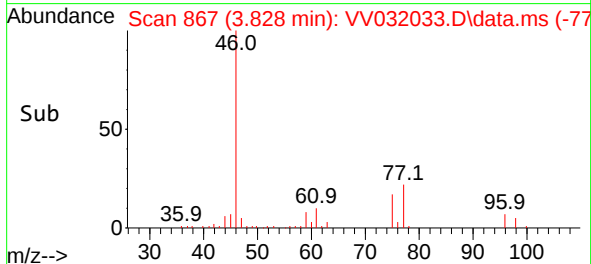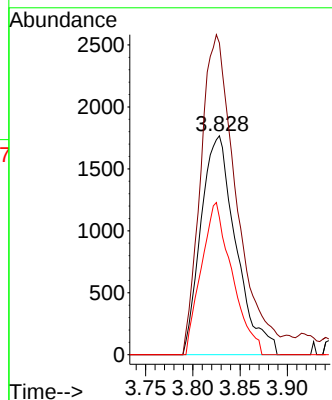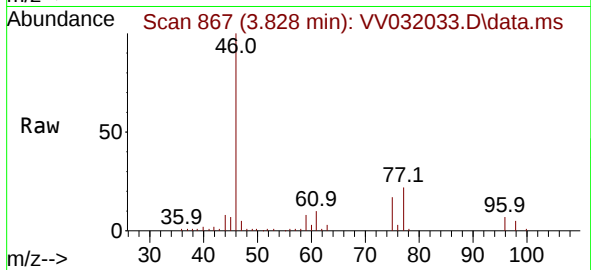

#34
Trichloroethene
Concen: 8.168 ug/L
RT: 5.838 min Scan# 1492
Delta R.T. 0.000 min
Lab File: VV032033.D
Acq: 11 Sep 2023 17:56

Tgt Ion: 95 Resp: 64342
Ion Ratio Lower Upper
95 100
97 64.7 47.7 88.7
132 91.4 63.8 118.4
130 95.1 68.7 127.5

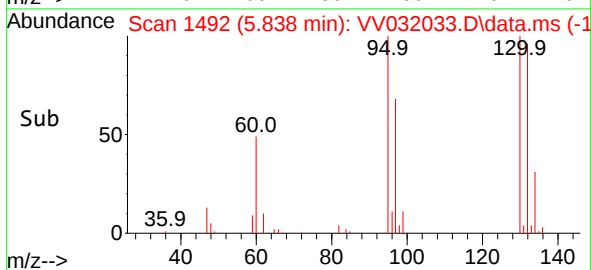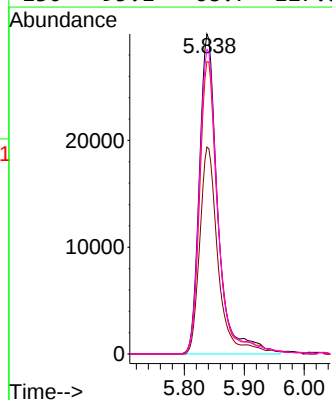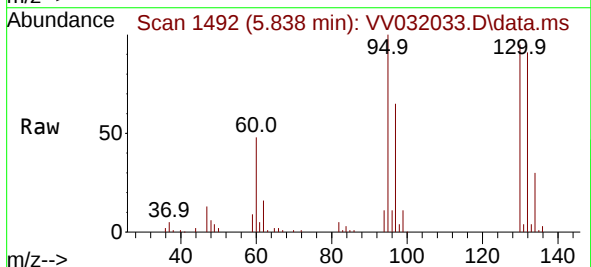

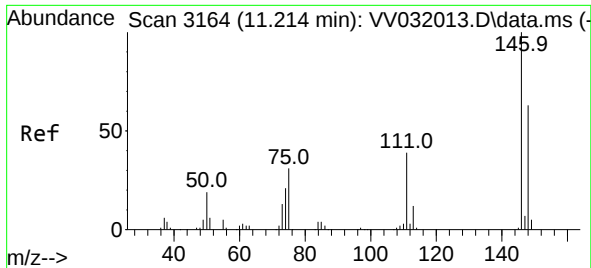

#65

1,4-Dichlorobenzene

Concen: 0.118 ug/L

RT: 11.214 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV032033.D


Acq: 11 Sep 2023 17:56

Instrument :

MSVOA_V

ClientSampleId :

BH4K9

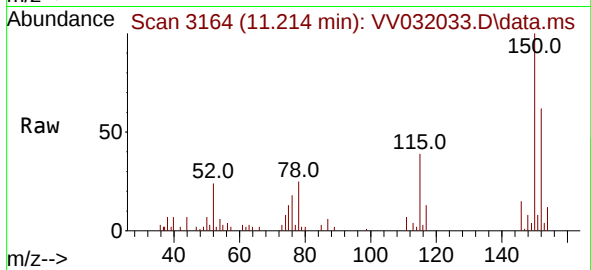

Tgt Ion:146 Resp: 1828

Ion Ratio Lower Upper

146 100

111 45.4 29.2 54.2

148 56.2 44.0 81.6

