

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032014.D
 Acq On : 11 Sep 2023 09:42
 Operator : SY/MD
 Sample : VV0911WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	34883	40139	7.43%	1.069%
2	1.532	146	153	167	rVB	41669	49613	9.18%	1.322%
3	2.060	308	317	331	rBV	69899	103345	19.13%	2.753%
4	3.809	852	861	897	rBV	48411	175555	32.49%	4.677%
5	4.253	982	999	1025	rBV	60036	154628	28.62%	4.119%
6	4.960	1203	1219	1245	rBV2	143445	367911	68.09%	9.801%
7	5.535	1386	1398	1423	rBV	183056	384047	71.07%	10.231%
8	5.831	1477	1490	1493	rBV10	4752	7719	1.43%	0.206%
9	5.992	1525	1540	1565	rBV	87002	186154	34.45%	4.959%
10	6.921	1819	1829	1849	rBV	31523	63582	11.77%	1.694%
11	7.246	1916	1930	1957	rBV	163186	302184	55.92%	8.050%
12	7.564	2018	2029	2045	rBV2	18396	37848	7.00%	1.008%
13	8.031	2165	2174	2211	rBV	215876	451008	83.46%	12.014%
14	8.789	2398	2410	2434	rBV	293428	496012	91.79%	13.213%
15	10.159	2825	2836	2849	rBV2	61803	100169	18.54%	2.668%
16	11.188	3145	3156	3175	rBV	343943	540364	100.00%	14.395%
17	11.564	3262	3273	3296	rBV	171979	276163	51.11%	7.357%
18	13.448	3849	3859	3874	rBV3	6732	11703	2.17%	0.312%
19	13.689	3925	3934	3945	rVB8	3685	5750	1.06%	0.153%




Sum of corrected areas: 3753894

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032014.D
Acq On : 11 Sep 2023 09:42
Operator : SY/MD
Sample : VV0911WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

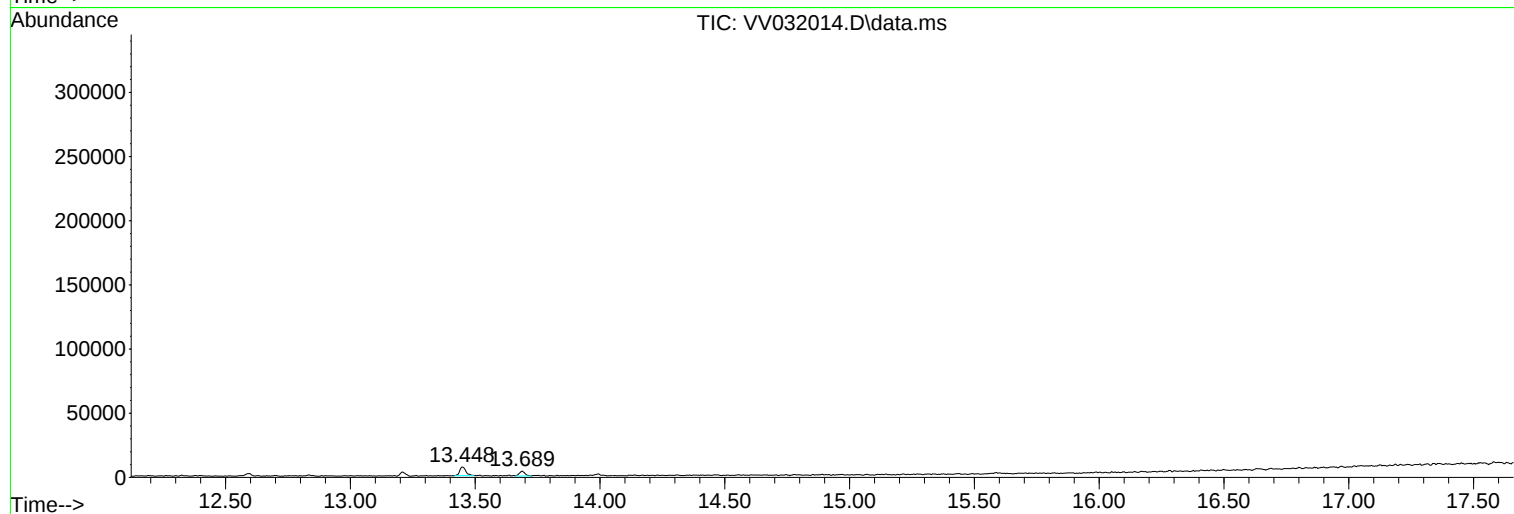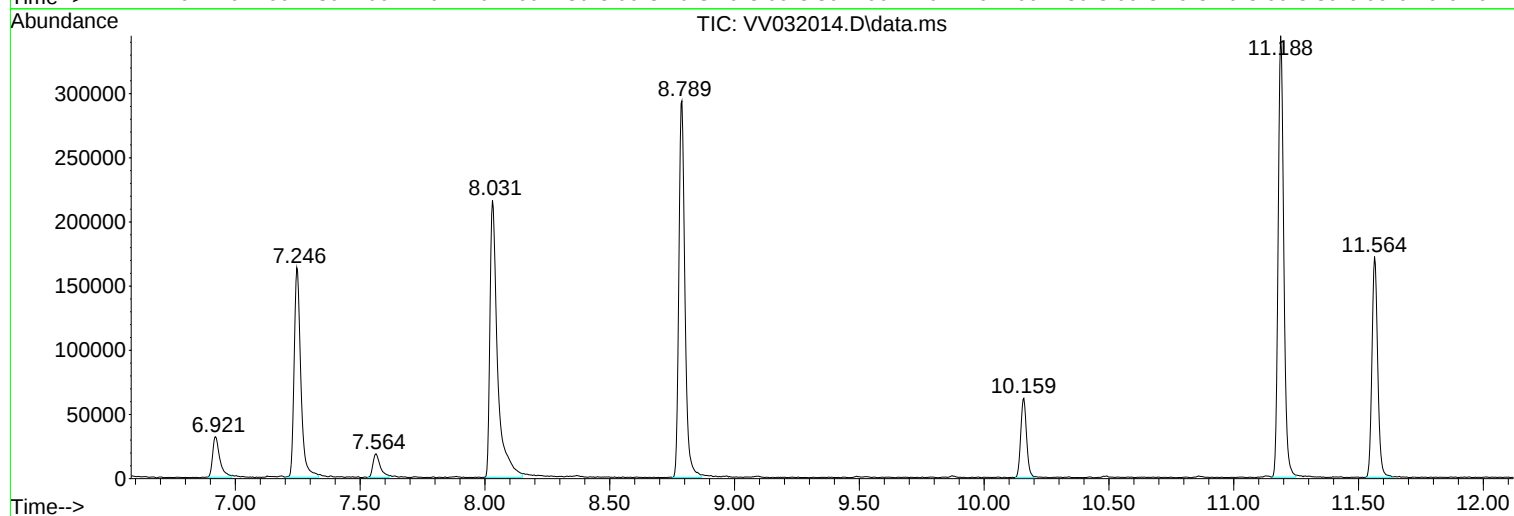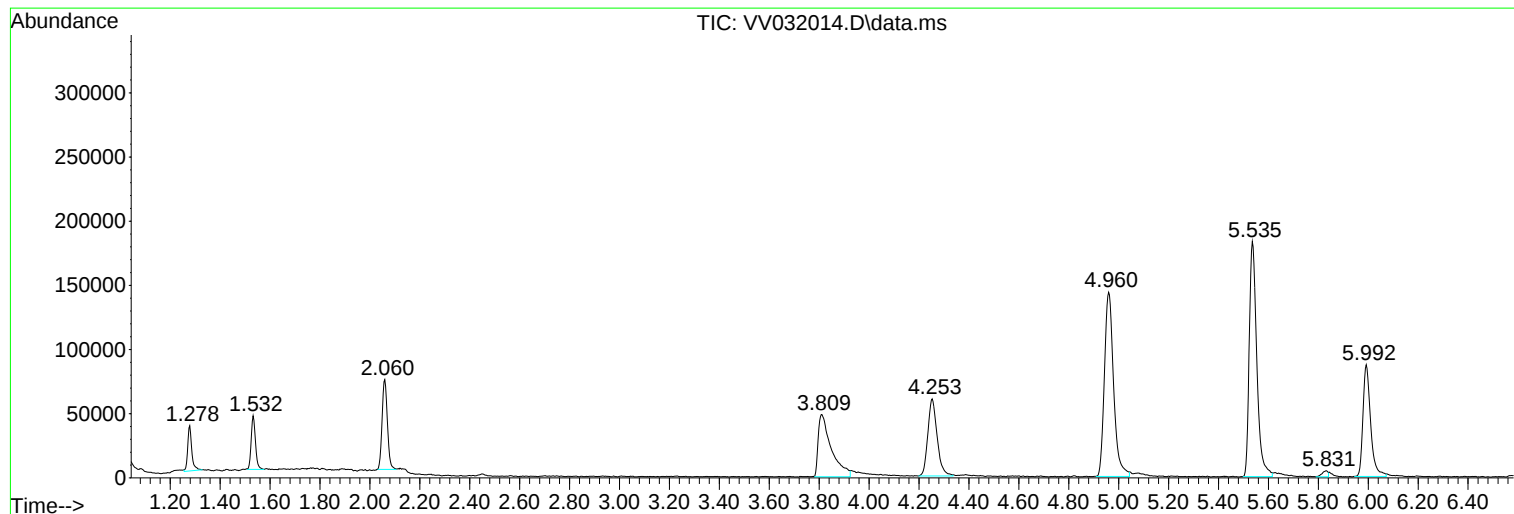

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032014.D
Acq On : 11 Sep 2023 09:42
Operator : SY/MD
Sample : VV0911WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032014.D
Acq On : 11 Sep 2023 09:42
Operator : SY/MD
Sample : VV0911WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------