

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032023.D
 Acq On : 11 Sep 2023 13:53
 Operator : SY/MD
 Sample : 04286-18DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4G3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	49	59	63	rBV9	2883	5284	1.09%	0.142%
2	1.278	67	74	86	rVV	33914	38611	7.97%	1.034%
3	1.532	146	153	167	rVB	42678	51657	10.67%	1.384%
4	2.060	307	317	329	rBV	72179	103773	21.43%	2.780%
5	2.449	429	438	453	rVB	9345	15912	3.29%	0.426%
6	3.822	852	865	916	rBV2	62518	251142	51.86%	6.727%
7	4.256	981	1000	1026	rBV	60011	161632	33.38%	4.330%
8	4.963	1205	1220	1249	rBV2	144556	378645	78.19%	10.142%
9	5.539	1387	1399	1423	rBV	137681	289799	59.85%	7.763%
10	5.838	1481	1492	1516	rBV2	82700	177120	36.58%	4.744%
11	5.995	1528	1541	1567	rBV	88342	190602	39.36%	5.106%
12	6.921	1816	1829	1849	rBV2	32024	66498	13.73%	1.781%
13	7.249	1915	1931	1961	rBV	165960	308980	63.81%	8.276%
14	7.564	2019	2029	2052	rBV	18790	36892	7.62%	0.988%
15	8.034	2164	2175	2216	rBV	228669	484243	100.00%	12.971%
16	8.789	2398	2410	2437	rBV	219331	379467	78.36%	10.164%
17	10.159	2822	2836	2854	rBV	65326	105256	21.74%	2.819%
18	11.191	3145	3157	3185	rBV	260011	409131	84.49%	10.959%
19	11.564	3262	3273	3296	rVB	173389	278622	57.54%	7.463%




Sum of corrected areas: 3733266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032023.D
Acq On : 11 Sep 2023 13:53
Operator : SY/MD
Sample : 04286-18DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4G3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

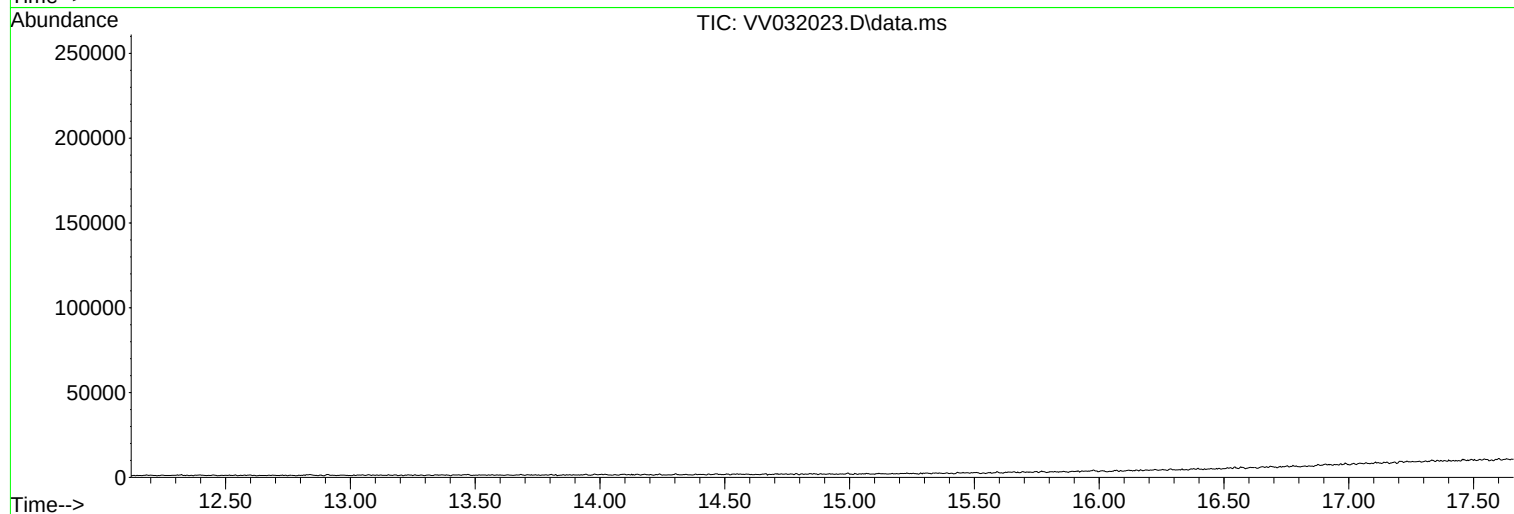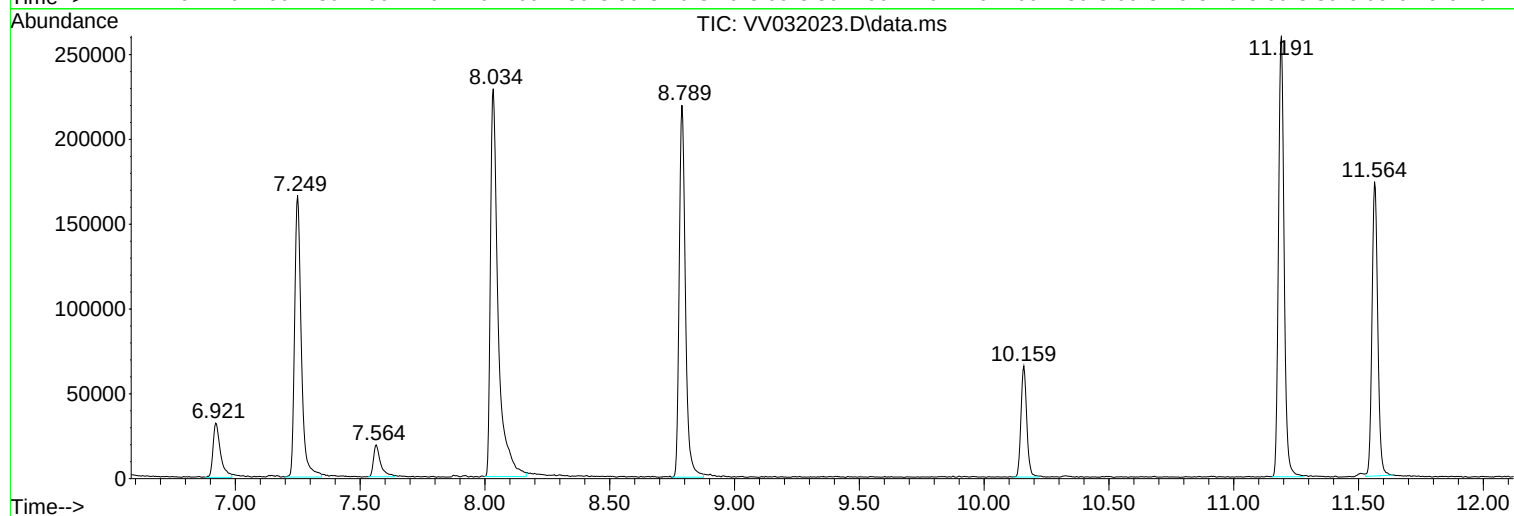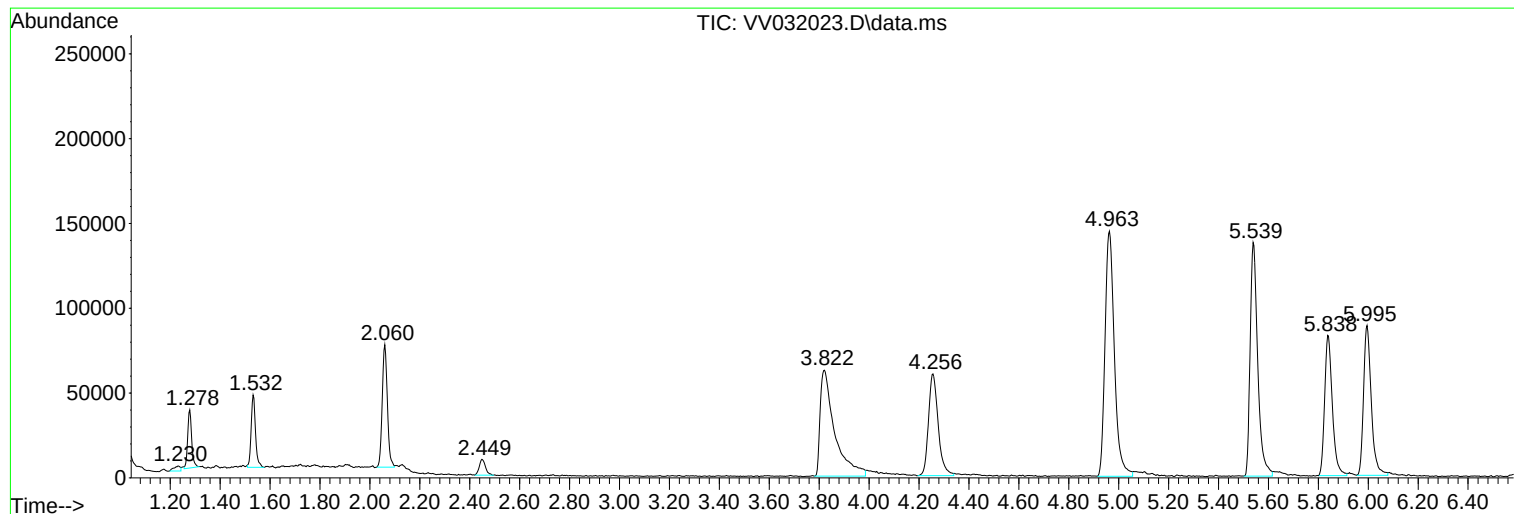

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032023.D
Acq On : 11 Sep 2023 13:53
Operator : SY/MD
Sample : 04286-18DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4G3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032023.D
Acq On : 11 Sep 2023 13:53
Operator : SY/MD
Sample : 04286-18DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4G3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc