

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032026.D
 Acq On : 11 Sep 2023 15:07
 Operator : SY/MD
 Sample : 04307-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4J3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	28648	30325	1.67%	0.472%
2	1.532	146	153	172	rVB	36547	44982	2.47%	0.701%
3	2.066	306	319	335	rBV4	137836	236032	12.96%	3.677%
4	2.703	505	517	529	rBV5	10255	22578	1.24%	0.352%
5	3.815	849	863	901	rBV2	542922	1385564	76.09%	21.586%
6	4.259	985	1001	1029	rBV2	53191	154848	8.50%	2.412%
7	4.963	1203	1220	1244	rBV2	123682	322113	17.69%	5.018%
8	5.538	1384	1399	1422	rBV	131699	282834	15.53%	4.406%
9	5.834	1476	1491	1529	rBV	887658	1820915	100.00%	28.368%
10	5.995	1530	1541	1561	rVB2	72582	155681	8.55%	2.425%
11	6.924	1820	1830	1847	rBV2	26480	53892	2.96%	0.840%
12	7.249	1920	1931	1964	rBV	138641	256355	14.08%	3.994%
13	7.564	2021	2029	2050	rBV2	15223	32454	1.78%	0.506%
14	7.911	2124	2137	2156	rBV	73544	130873	7.19%	2.039%
15	8.030	2164	2174	2216	rBV	198124	413752	22.72%	6.446%
16	8.789	2399	2410	2435	rBV	207533	358350	19.68%	5.583%
17	10.159	2826	2836	2856	rBV	55637	90553	4.97%	1.411%
18	11.191	3145	3157	3179	rBV	246615	392125	21.53%	6.109%
19	11.567	3263	3274	3289	rBV	146569	234728	12.89%	3.657%




Sum of corrected areas: 6418954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032026.D
Acq On : 11 Sep 2023 15:07
Operator : SY/MD
Sample : 04307-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

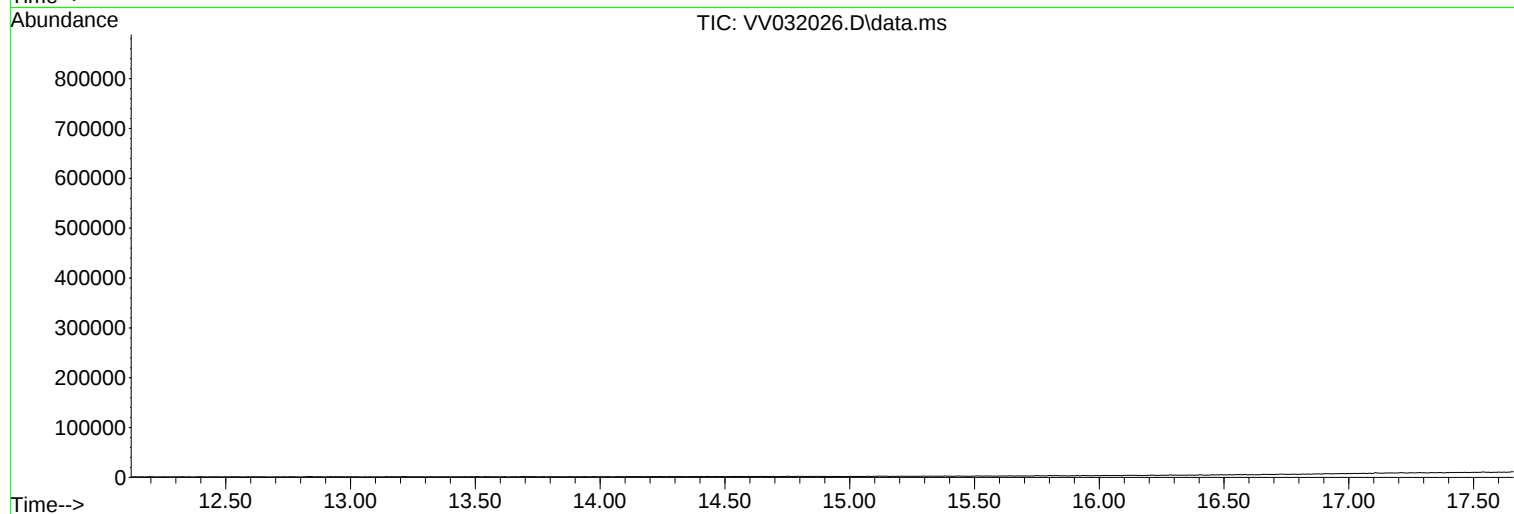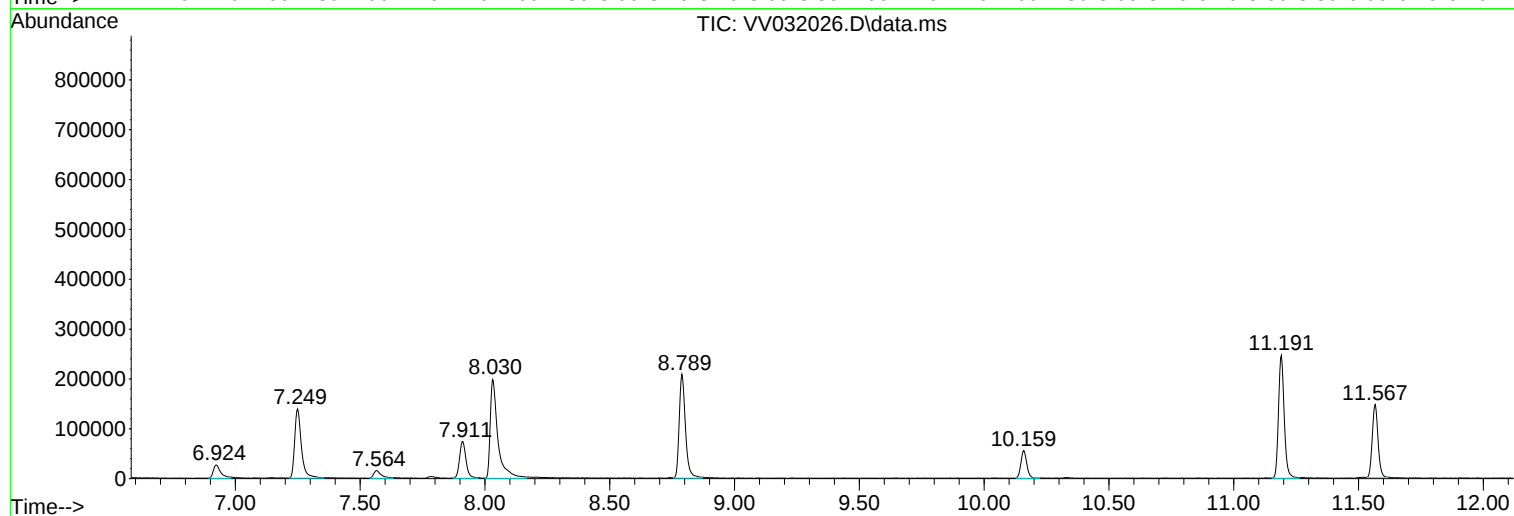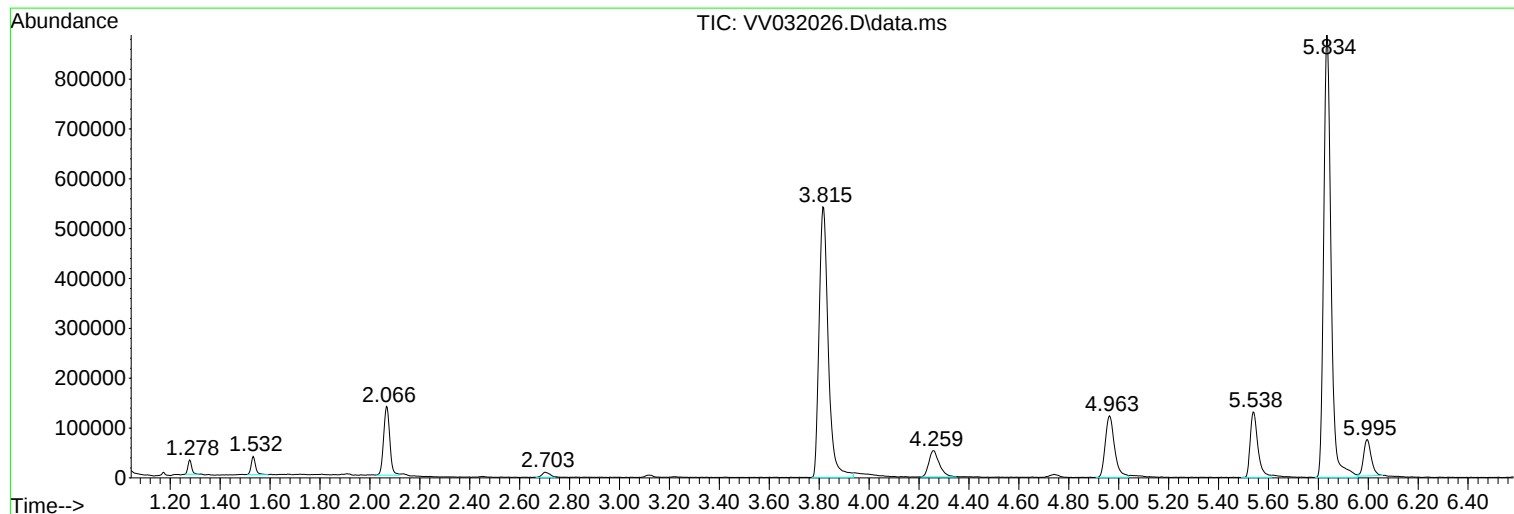

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032026.D
Acq On : 11 Sep 2023 15:07
Operator : SY/MD
Sample : 04307-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032026.D
Acq On : 11 Sep 2023 15:07
Operator : SY/MD
Sample : 04307-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc