

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032031.D
 Acq On : 11 Sep 2023 17:07
 Operator : SY/MD
 Sample : 04306-09 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	82	rBV	29380	31832	5.52%	0.784%
2	1.532	146	153	161	rBV	34346	39952	6.93%	0.984%
3	2.060	308	317	335	rBV	58061	89748	15.56%	2.211%
4	2.452	429	439	449	rBV	6783	12618	2.19%	0.311%
5	2.709	503	519	542	rBV	271071	576742	100.00%	14.207%
6	3.818	842	864	902	rBV2	70129	238281	41.32%	5.870%
7	4.256	983	1000	1019	rBV2	50362	132799	23.03%	3.271%
8	4.963	1206	1220	1240	rBV3	123392	314326	54.50%	7.743%
9	5.542	1388	1400	1423	rBV	130902	278129	48.22%	6.851%
10	5.838	1479	1492	1511	rBV	158755	329820	57.19%	8.124%
11	5.995	1529	1541	1567	rBV	74284	158429	27.47%	3.903%
12	6.924	1820	1830	1845	rBV	26480	53933	9.35%	1.329%
13	7.249	1918	1931	1950	rBV	134873	253455	43.95%	6.243%
14	7.567	2018	2030	2050	rBV2	15985	34867	6.05%	0.859%
15	7.915	2130	2138	2148	rVB5	5659	10114	1.75%	0.249%
16	8.034	2164	2175	2211	rBV	204259	426276	73.91%	10.500%
17	8.789	2397	2410	2435	rBV	208963	359700	62.37%	8.860%
18	10.159	2823	2836	2853	rBV	57521	92401	16.02%	2.276%
19	11.191	3146	3157	3179	rBV	249607	388777	67.41%	9.577%
20	11.564	3262	3273	3291	rBV	145153	237403	41.16%	5.848%




Sum of corrected areas: 4059602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032031.D
Acq On : 11 Sep 2023 17:07
Operator : SY/MD
Sample : 04306-09 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

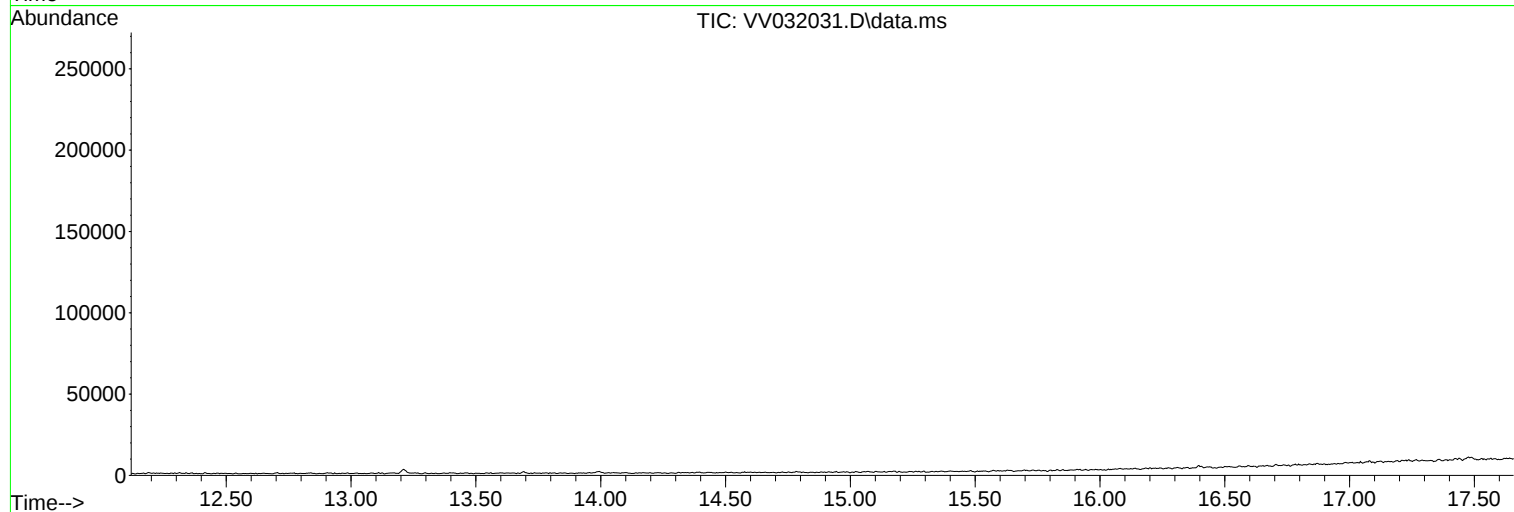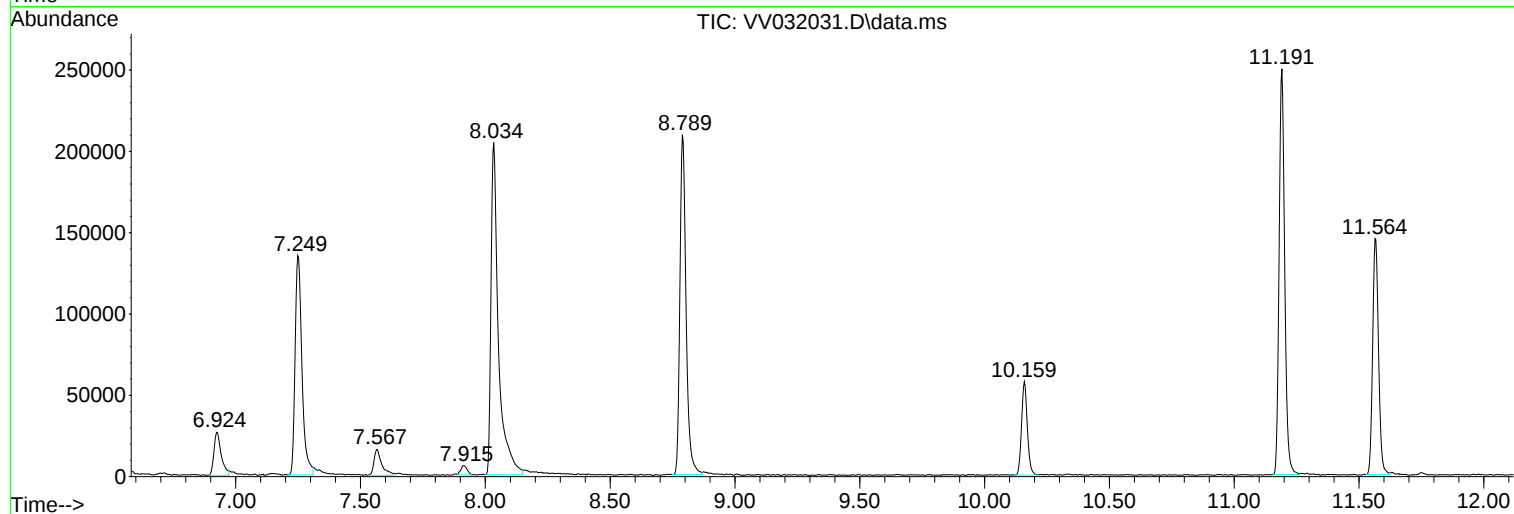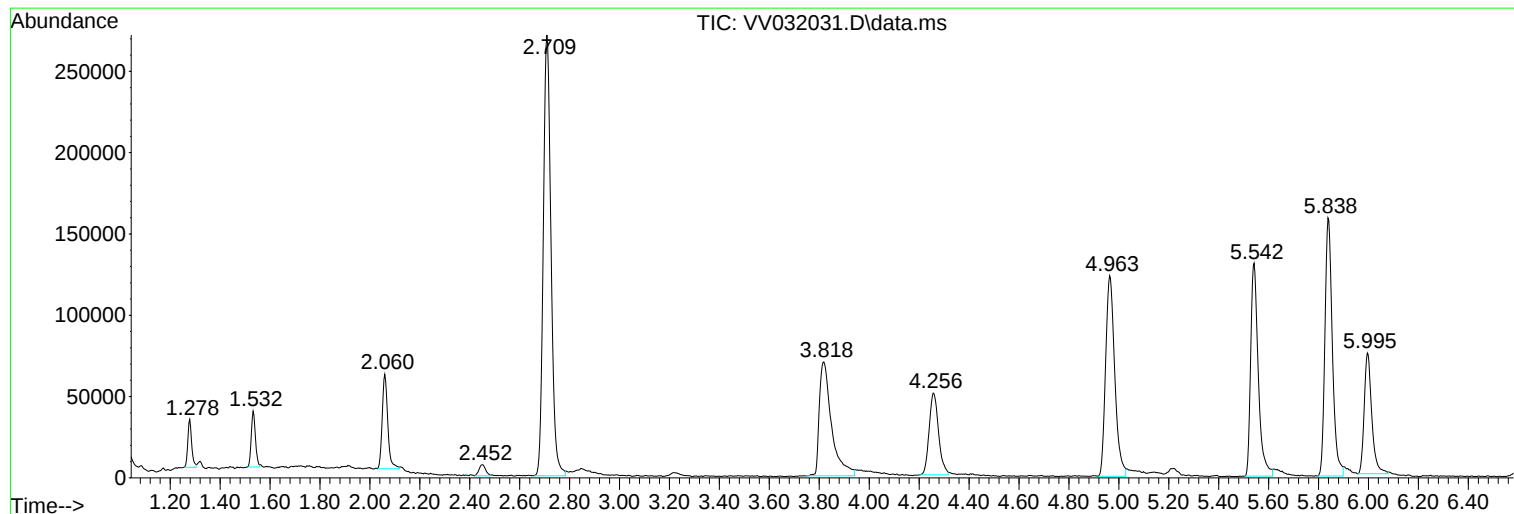

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032031.D
Acq On : 11 Sep 2023 17:07
Operator : SY/MD
Sample : 04306-09 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032031.D
Acq On : 11 Sep 2023 17:07
Operator : SY/MD
Sample : 04306-09 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------