

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032032.D
 Acq On : 11 Sep 2023 17:32
 Operator : SY/MD
 Sample : 04306-12 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4K7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	27943	29555	7.05%	0.860%
2	1.532	146	153	162	rVB	33482	38252	9.12%	1.113%
3	2.060	308	317	333	rBV	56354	83786	19.98%	2.437%
4	2.452	429	439	454	rVB4	6097	12043	2.87%	0.350%
5	2.709	507	519	537	rVB2	17021	36316	8.66%	1.056%
6	3.815	850	863	899	rBV2	57142	212544	50.68%	6.182%
7	4.256	984	1000	1028	rBV	49985	135868	32.40%	3.952%
8	4.963	1204	1220	1238	rBV3	120955	306945	73.19%	8.928%
9	5.539	1387	1399	1423	rBV2	130799	281879	67.21%	8.199%
10	5.838	1478	1492	1516	rBV	140285	298167	71.10%	8.673%
11	5.995	1528	1541	1557	rBV	72812	155323	37.04%	4.518%
12	6.924	1820	1830	1854	rBV	24644	55010	13.12%	1.600%
13	7.249	1920	1931	1960	rBV	134768	255199	60.85%	7.423%
14	7.564	2021	2029	2054	rBV2	14796	31651	7.55%	0.921%
15	7.918	2131	2139	2148	rVB4	3201	5685	1.36%	0.165%
16	8.034	2165	2175	2210	rBV	199379	419374	100.00%	12.198%
17	8.789	2398	2410	2441	rBV	210830	366214	87.32%	10.652%
18	10.159	2822	2836	2854	rBV	55975	91627	21.85%	2.665%
19	11.191	3146	3157	3175	rBV	243577	392704	93.64%	11.423%
20	11.564	3262	3273	3294	rBV	140128	229778	54.79%	6.684%




Sum of corrected areas: 3437920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032032.D
Acq On : 11 Sep 2023 17:32
Operator : SY/MD
Sample : 04306-12 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

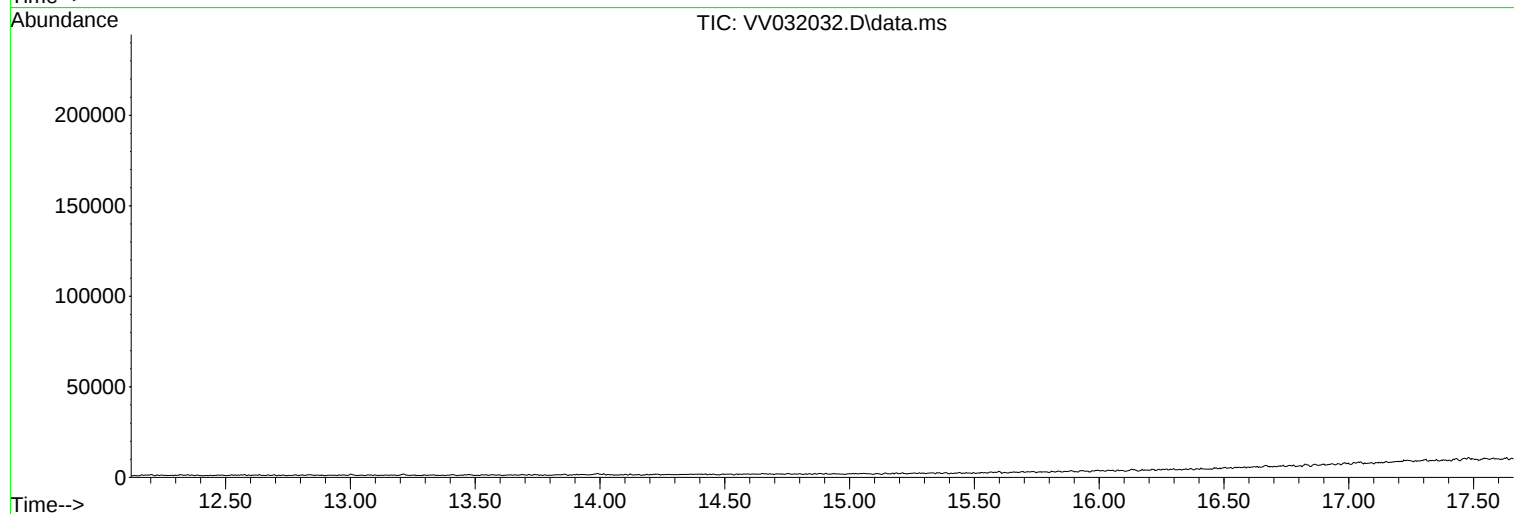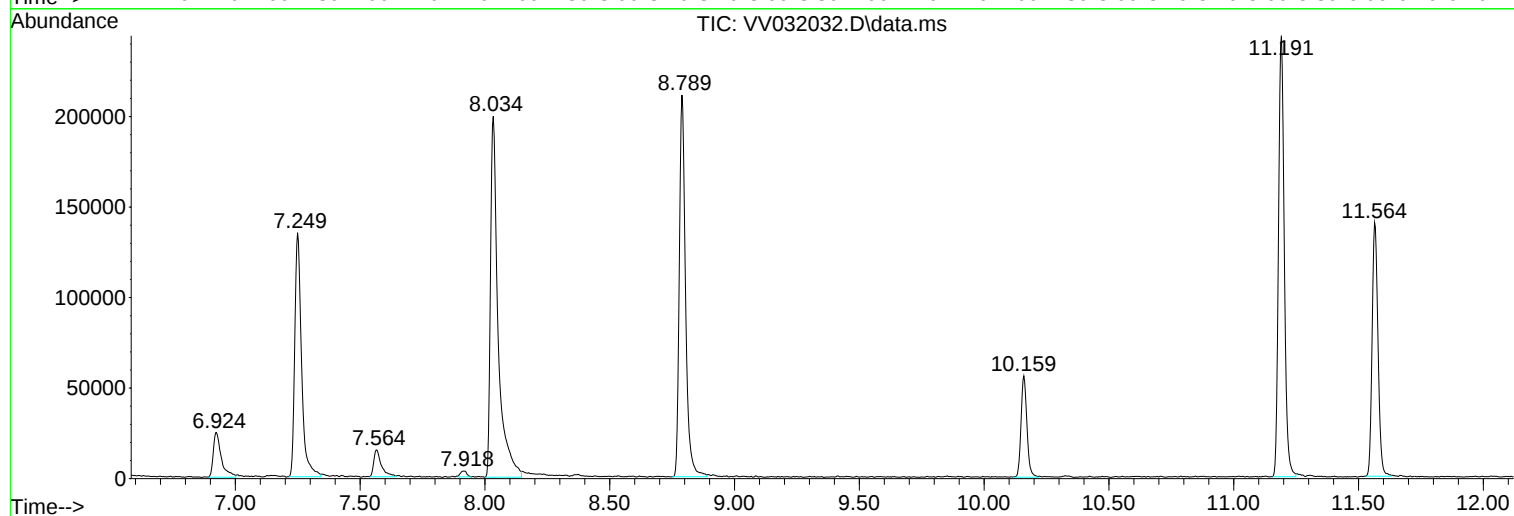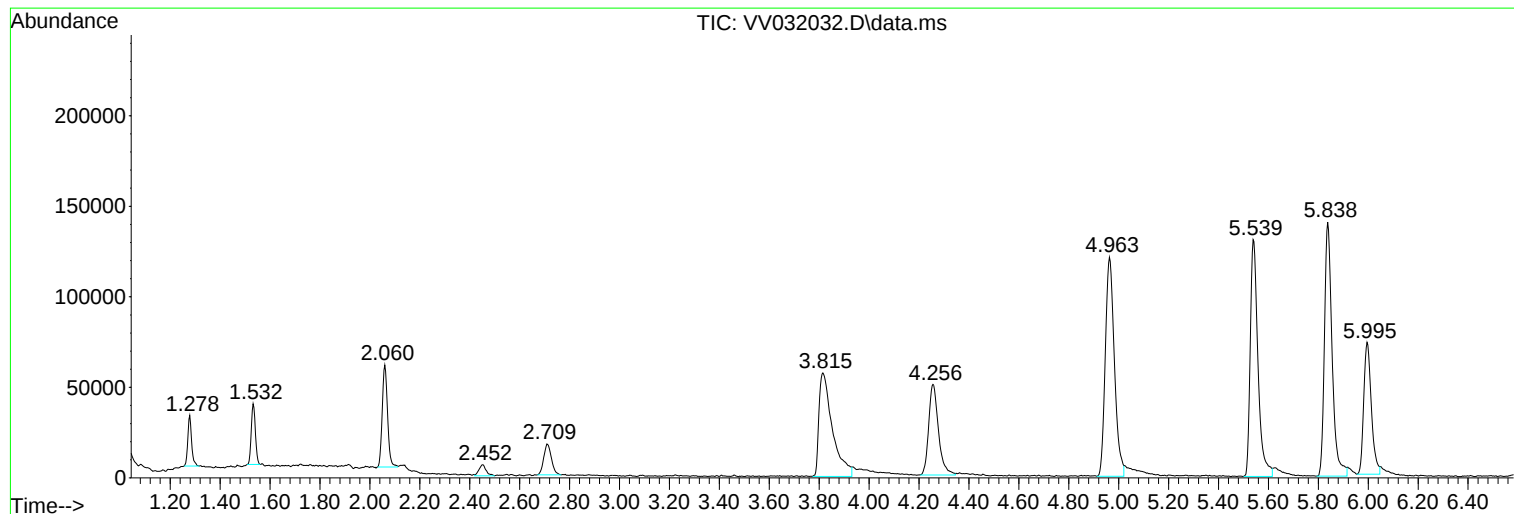

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032032.D
Acq On : 11 Sep 2023 17:32
Operator : SY/MD
Sample : 04306-12 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032032.D
Acq On : 11 Sep 2023 17:32
Operator : SY/MD
Sample : 04306-12 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------