

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032033.D
 Acq On : 11 Sep 2023 17:56
 Operator : SY/MD
 Sample : 04306-13 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4K9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	28873	31814	7.35%	0.909%
2	1.532	146	153	165	rVB	35563	42488	9.82%	1.214%
3	2.060	307	317	331	rBV	57940	85118	19.67%	2.432%
4	2.449	427	438	448	rBV	6664	10730	2.48%	0.307%
5	2.712	512	520	529	rBV5	2953	5785	1.34%	0.165%
6	3.818	851	864	900	rBV3	55703	206803	47.79%	5.908%
7	4.256	985	1000	1026	rBV	51096	137417	31.76%	3.926%
8	4.963	1203	1220	1245	rBV2	122324	319836	73.91%	9.137%
9	5.542	1387	1400	1422	rBV	128183	277726	64.18%	7.934%
10	5.838	1479	1492	1513	rBV	166875	350820	81.07%	10.022%
11	5.995	1529	1541	1557	rBV	74571	156364	36.14%	4.467%
12	6.924	1819	1830	1852	rBV2	25376	56146	12.98%	1.604%
13	7.249	1920	1931	1965	rBV	137160	258207	59.67%	7.376%
14	7.564	2021	2029	2048	rBV	15327	31808	7.35%	0.909%
15	8.034	2165	2175	2219	rBV	200425	432717	100.00%	12.361%
16	8.789	2399	2410	2434	rBV	211387	367425	84.91%	10.496%
17	10.159	2824	2836	2853	rBV	57201	93000	21.49%	2.657%
18	11.191	3146	3157	3175	rBV	248263	395879	91.49%	11.309%
19	11.567	3260	3274	3290	rBV	149375	240453	55.57%	6.869%




Sum of corrected areas: 3500536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032033.D
Acq On : 11 Sep 2023 17:56
Operator : SY/MD
Sample : 04306-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

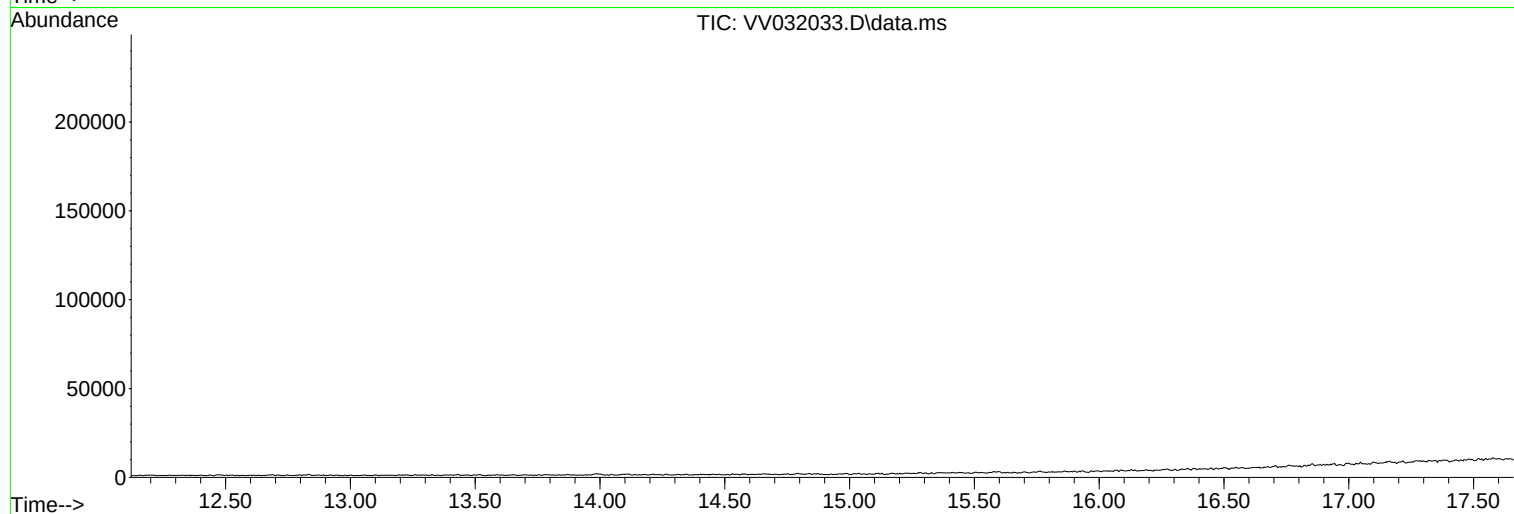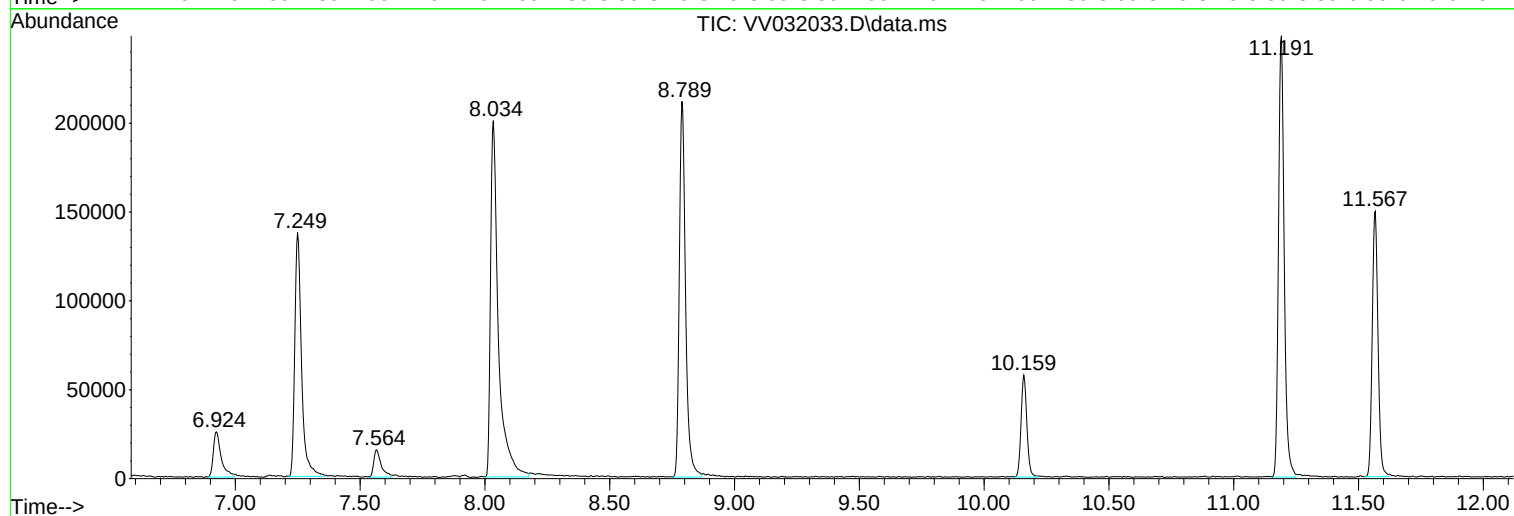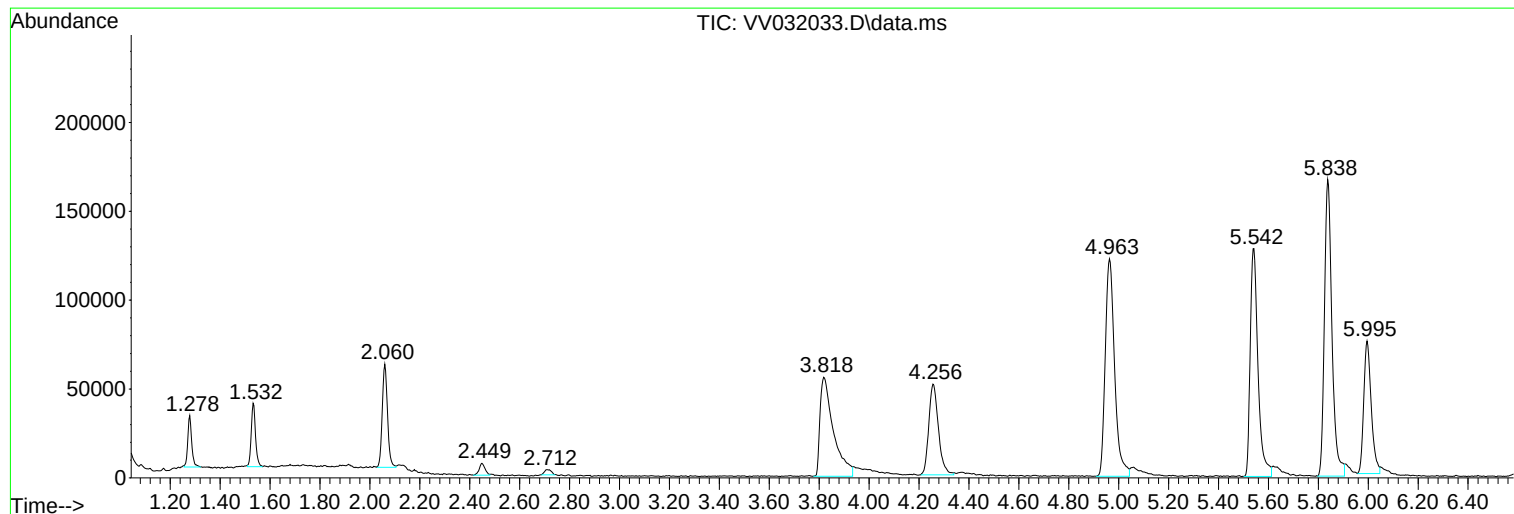

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032033.D
Acq On : 11 Sep 2023 17:56
Operator : SY/MD
Sample : 04306-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032033.D
Acq On : 11 Sep 2023 17:56
Operator : SY/MD
Sample : 04306-13 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4K9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc