

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032036.D
 Acq On : 11 Sep 2023 19:10
 Operator : SY/MD
 Sample : 04306-16 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH4L2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	83	rVB	28481	30159	2.65%	0.671%
2	1.532	146	153	164	rBV	37536	43796	3.84%	0.975%
3	2.060	308	317	332	rBV	60334	89013	7.81%	1.981%
4	2.452	427	439	449	rBV3	6544	12179	1.07%	0.271%
5	3.815	847	863	894	rBV2	100324	313429	27.51%	6.975%
6	4.256	982	1000	1024	rBV	53410	144466	12.68%	3.215%
7	4.963	1205	1220	1243	rBV2	128319	330819	29.04%	7.362%
8	5.539	1388	1399	1422	rBV	131503	281398	24.70%	6.262%
9	5.834	1478	1491	1508	rBV	569655	1139252	100.00%	25.351%
10	5.995	1529	1541	1571	rVB	77084	170060	14.93%	3.784%
11	6.924	1818	1830	1850	rBV2	26806	58626	5.15%	1.305%
12	7.249	1918	1931	1962	rBV	145527	273191	23.98%	6.079%
13	7.564	2020	2029	2050	rBV2	15416	33360	2.93%	0.742%
14	7.915	2126	2138	2150	rVB5	7155	12930	1.13%	0.288%
15	8.030	2162	2174	2210	rBV	212491	448434	39.36%	9.979%
16	8.789	2398	2410	2434	rBV	215385	368528	32.35%	8.201%
17	10.159	2825	2836	2852	rBV	61239	97786	8.58%	2.176%
18	11.191	3146	3157	3182	rBV	250196	397474	34.89%	8.845%
19	11.564	3261	3273	3296	rBV	153670	248927	21.85%	5.539%




Sum of corrected areas: 4493827

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032036.D
Acq On : 11 Sep 2023 19:10
Operator : SY/MD
Sample : 04306-16 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

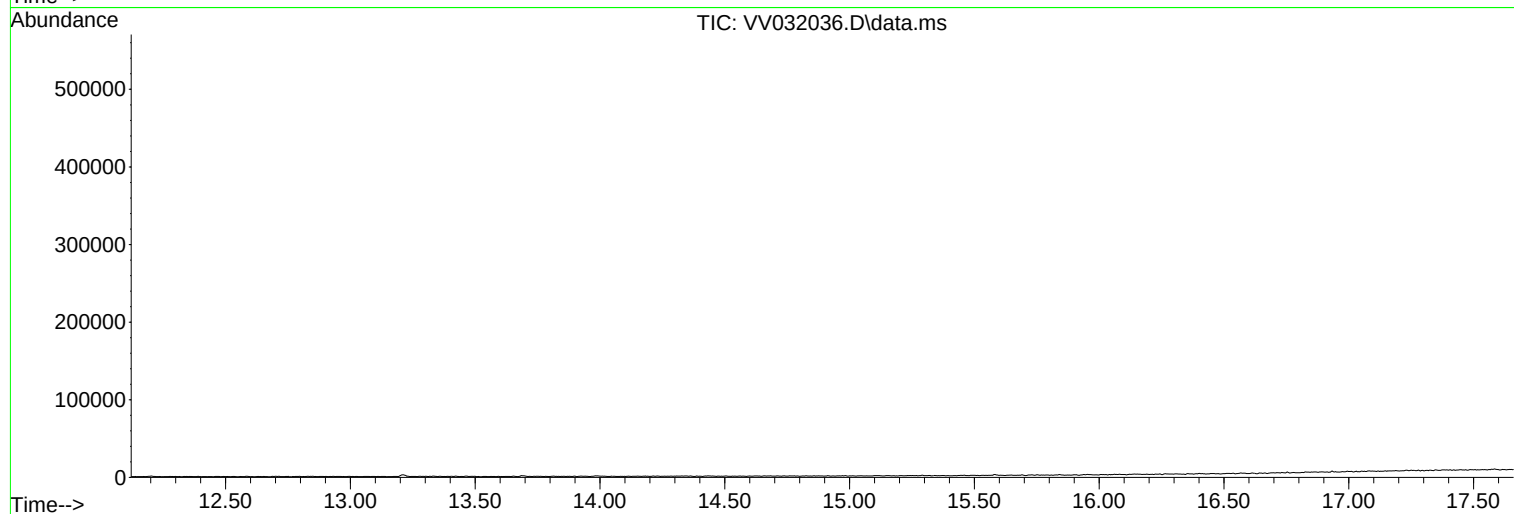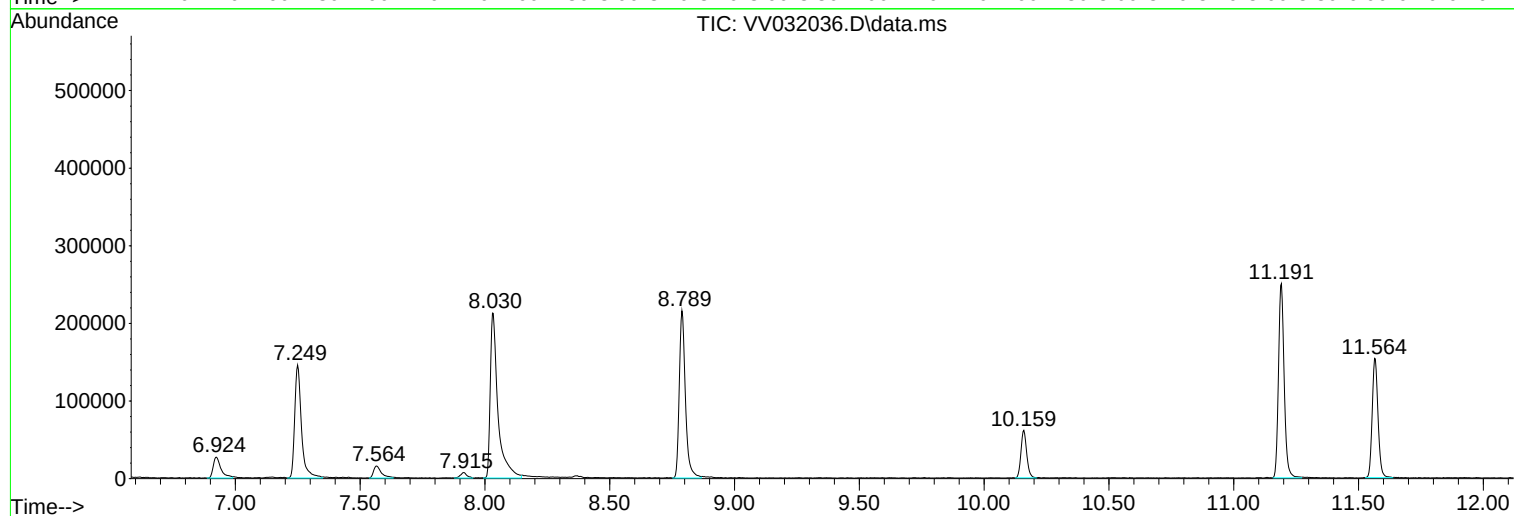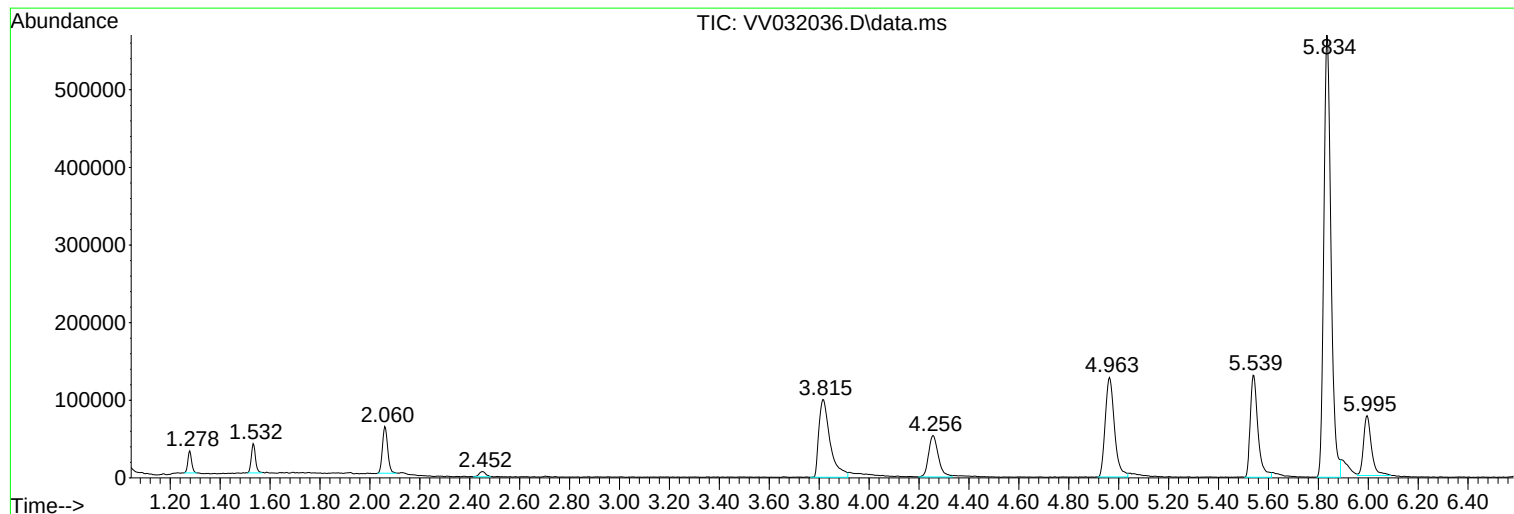

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032036.D
Acq On : 11 Sep 2023 19:10
Operator : SY/MD
Sample : 04306-16 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
Data File : VV032036.D
Acq On : 11 Sep 2023 19:10
Operator : SY/MD
Sample : 04306-16 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH4L2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc