
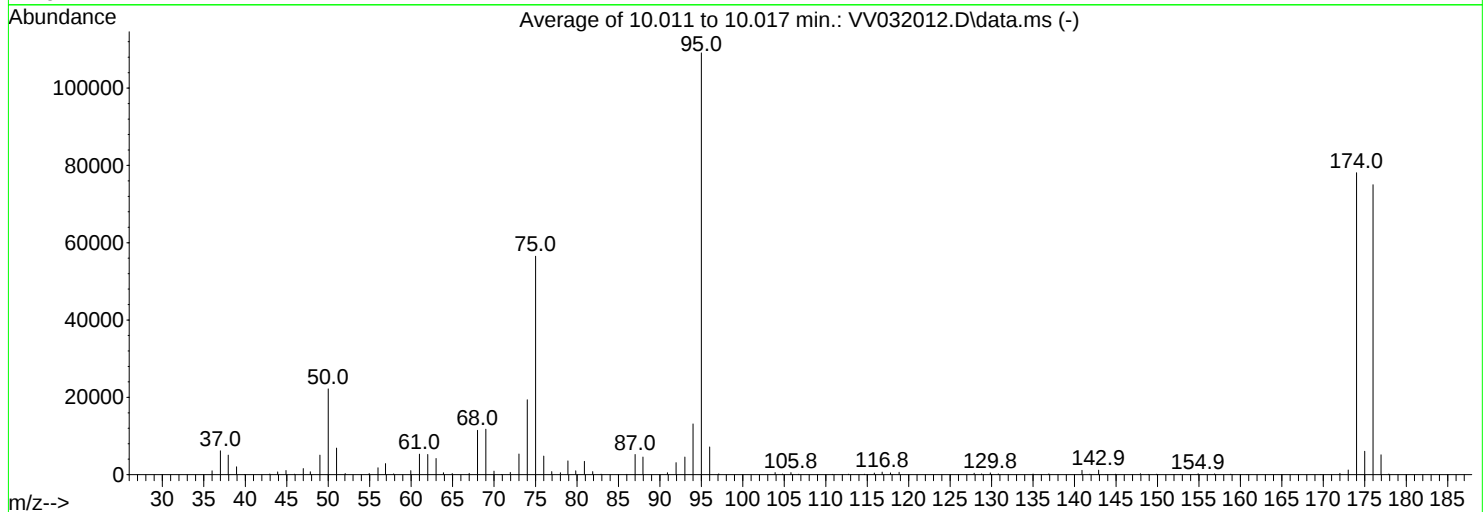


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091123\
 Data File : VV032012.D
 Acq On : 11 Sep 2023 08:39
 Operator : SY/MD
 Sample : BFB290
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB290

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR082323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Sep 09 21:51:31 2023

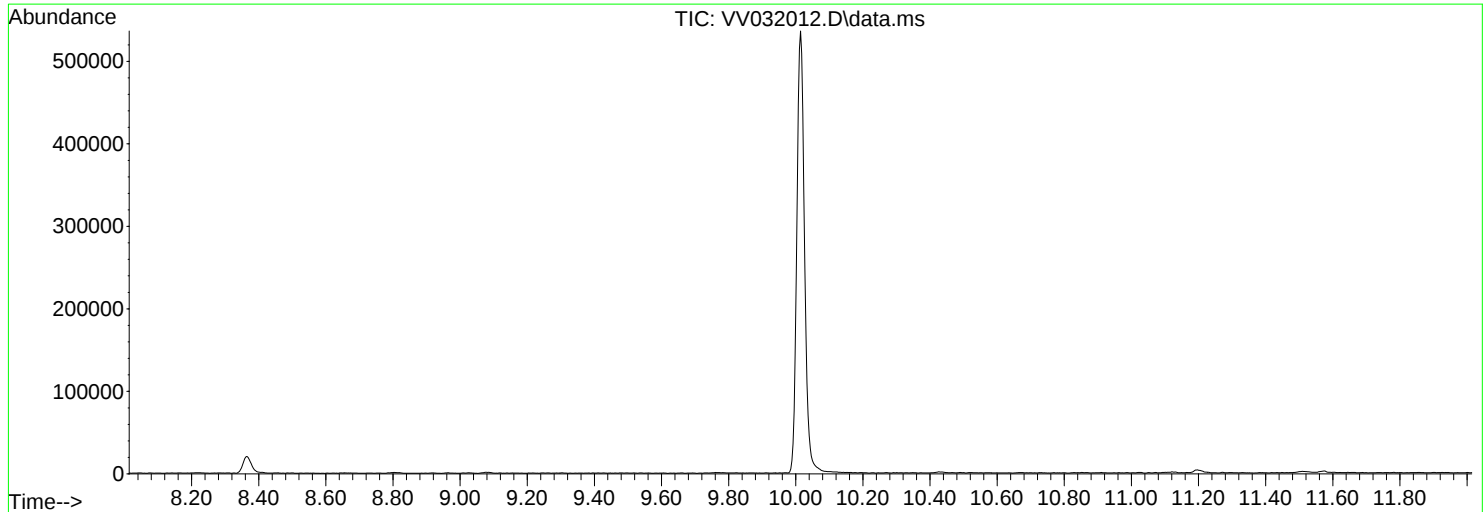

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	22189	PASS
75	95	30	80	51.8	56525	PASS
95	95	100	100	100.0	109128	PASS
96	95	5	9	6.6	7161	PASS
173	174	0.00	2	1.5	1190	PASS
174	95	50	120	71.6	78117	PASS
175	174	5	9	7.7	6042	PASS
176	174	95	105	96.0	75003	PASS
177	176	5	10	6.8	5124	PASS

m/z	Abundance
36.10	100.0
37.80	102.0
38.90	139.0
40.00	243.0
41.00	152.0
43.90	522.0
56.80	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	1077.0
37.00	6178.0
38.00	5160.0
39.00	2122.0
39.90	276.0
40.90	122.0
42.90	160.0
43.90	1243.0
44.90	1057.0
45.90	139.0
47.00	1693.0
47.80	697.0
49.00	5084.0
50.00	22568.0
51.00	6743.0
52.10	310.0
54.90	311.0
56.00	1878.0
56.90	3046.0
57.90	187.0
60.00	996.0
61.00	5315.0
62.00	5370.0
63.00	4310.0
63.90	554.0
65.00	265.0
67.00	350.0
68.00	11494.0
69.00	11850.0
70.00	926.0
70.90	105.0
71.90	599.0
73.00	5341.0
74.00	19408.0
75.00	56656.0
76.00	4844.0
77.00	787.0
78.00	532.0
78.90	3555.0
79.80	992.0
80.90	3373.0
81.90	815.0
82.90	128.0
87.00	5218.0
88.00	4692.0
90.90	479.0
92.00	3039.0
93.00	4519.0
94.00	13077.0
95.00	108144.0
96.00	7206.0
97.10	244.0
103.90	493.0
104.80	131.0
105.80	491.0
106.70	119.0
110.80	122.0
112.80	109.0
114.60	144.0
115.90	376.0
116.80	650.0
117.80	448.0
118.90	580.0
127.90	335.0
128.80	244.0
129.80	435.0
130.80	196.0
135.00	146.0
136.90	238.0
140.90	1068.0
141.80	159.0
142.90	1128.0
143.80	111.0
144.90	146.0
148.00	232.0
148.90	119.0
149.90	109.0
155.00	224.0
156.90	207.0
158.80	124.0
172.00	347.0
173.00	1119.0
174.00	75880.0
175.00	5727.0
176.00	72464.0
176.90	4972.0
177.90	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	1135.0
37.00	6384.0
38.00	5278.0
39.00	2223.0
39.90	284.0
40.80	125.0
42.90	177.0
43.90	1237.0
44.90	1110.0
45.90	143.0
47.00	1643.0
47.90	754.0
49.00	5215.0
50.00	22904.0
51.00	7097.0
52.10	308.0
54.90	310.0
56.00	1885.0
56.90	3054.0
57.90	202.0
60.00	1083.0
61.00	5416.0
62.00	5371.0
63.00	4352.0
63.90	531.0
65.00	291.0
67.00	335.0
68.00	11912.0
69.00	12114.0
70.00	950.0
72.00	615.0
73.00	5507.0
74.00	19944.0
75.00	58032.0
76.00	5017.0
77.00	830.0
78.00	524.0
78.90	3710.0
79.90	1037.0
80.90	3537.0
81.90	802.0
82.90	134.0
87.00	5370.0
88.00	4640.0
90.90	498.0
92.00	3226.0
93.00	4742.0
94.00	13430.0
95.00	112608.0
96.00	7488.0
97.10	212.0
103.90	569.0
104.80	161.0
105.80	568.0
106.70	134.0
110.80	122.0
112.70	116.0
114.60	136.0
115.80	422.0
116.80	661.0
117.80	455.0
118.80	650.0
127.90	387.0
128.80	233.0
129.80	462.0
130.80	237.0
135.00	168.0
136.90	226.0
140.90	1172.0
141.90	132.0
142.90	1254.0
144.90	141.0
147.90	241.0
148.90	114.0
149.90	133.0
152.00	104.0
152.80	111.0
154.90	242.0
156.90	232.0
158.80	117.0
169.70	104.0
172.00	355.0
173.00	1254.0
174.00	80544.0
175.00	6233.0
176.00	77416.0
176.90	5287.0
177.90	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	1062.0
37.00	5906.0
38.00	4968.0
39.00	2122.0
39.90	303.0
40.80	106.0
43.00	179.0
44.00	1219.0
44.90	1045.0
46.00	127.0
47.00	1427.0
47.90	762.0
49.00	4918.0
50.00	21096.0
51.00	6768.0
52.00	311.0
55.00	301.0
56.00	1612.0
57.00	2891.0
57.90	196.0
59.90	1071.0
61.00	5173.0
62.00	4904.0
63.00	3932.0
63.90	448.0
64.90	268.0
67.00	297.0
68.00	11038.0
69.00	11292.0
70.00	878.0
72.00	587.0
73.00	5131.0
74.00	18768.0
75.00	54888.0
76.00	4568.0
76.90	813.0
78.00	475.0
78.90	3485.0
79.90	991.0
80.90	3370.0
81.90	706.0
82.90	122.0
86.00	218.0
87.00	5035.0
87.90	4340.0
90.90	476.0
91.90	3043.0
93.00	4351.0
94.00	12833.0
95.00	106632.0
96.00	6789.0
97.10	195.0
103.90	545.0
104.80	185.0
105.80	551.0
106.80	120.0
112.70	120.0
114.70	116.0
115.80	404.0
116.80	654.0
117.80	420.0
118.80	669.0
127.90	400.0
128.80	204.0
129.90	415.0
130.80	239.0
135.00	174.0
136.90	188.0
140.90	1120.0
141.90	104.0
142.90	1152.0
145.00	136.0
147.90	239.0
149.90	154.0
152.80	110.0
154.80	251.0
156.90	208.0
158.90	129.0
160.80	122.0
172.00	346.0
173.00	1198.0
174.00	77928.0
175.00	6167.0
176.00	75128.0
177.00	5114.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290