


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091125\
Data File : VV039037.D
Acq On : 11 Sep 2025 10:07
Operator : SY/MD
Sample : BFB205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM091125WMA.M
Title : VOC Analysis
Last Update : Fri Sep 12 01:49:00 2025

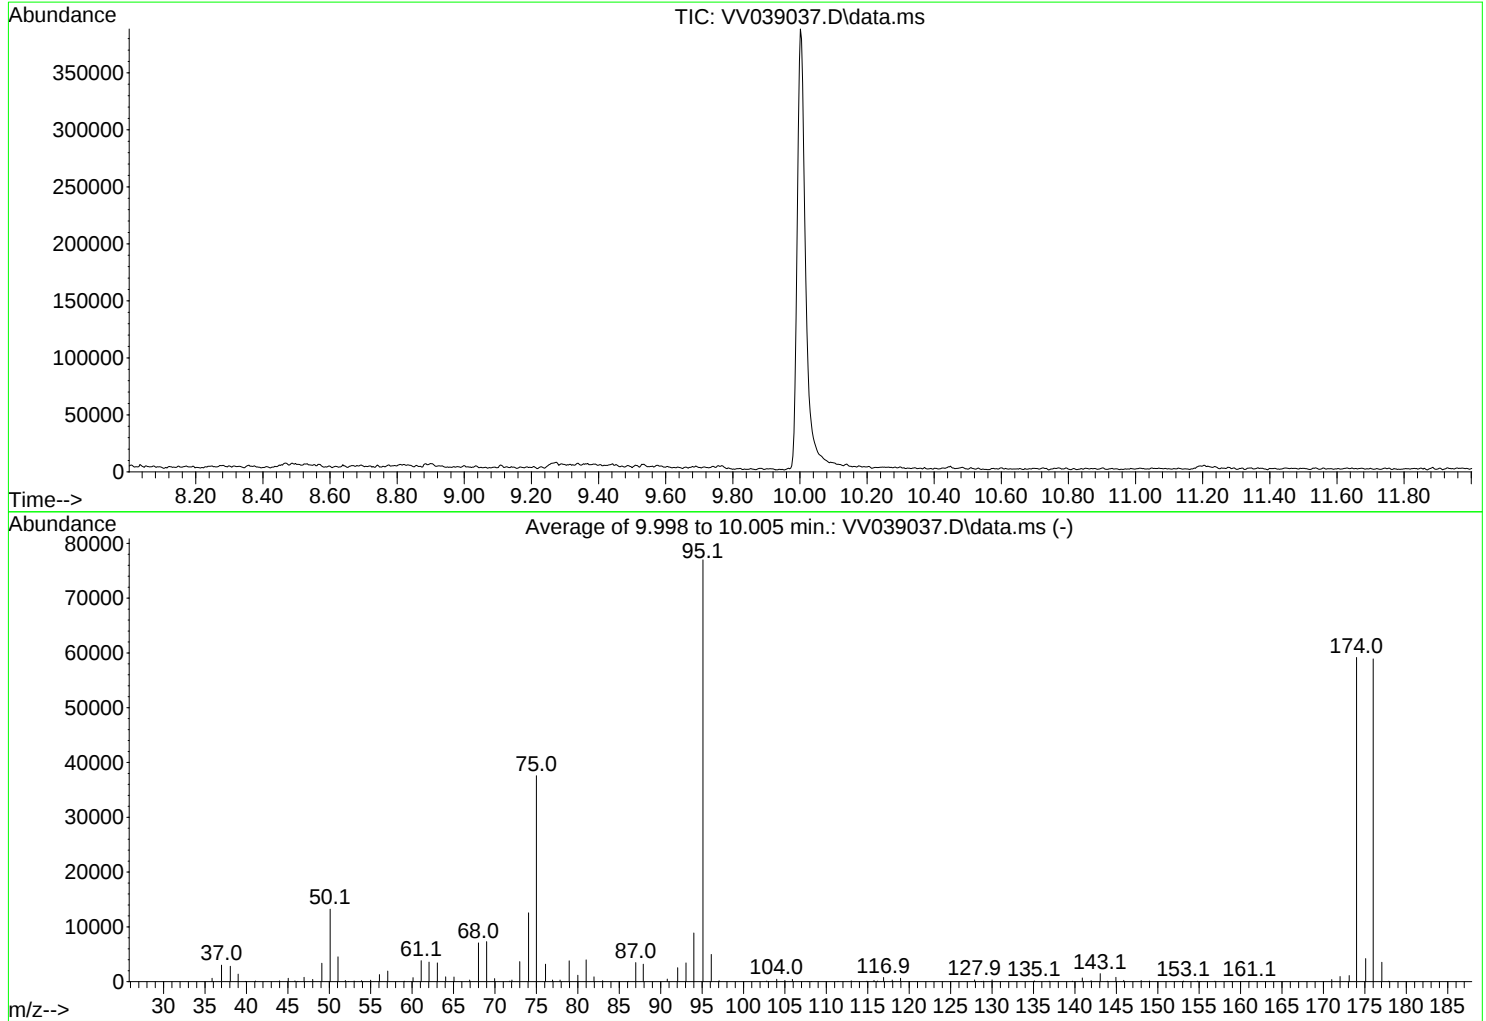

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	13228	PASS
75	95	30	80	48.8	37576	PASS
95	95	100	100	100.0	76987	PASS
96	95	5	9	6.5	4969	PASS
173	174	0.00	2	1.9	1123	PASS
174	95	50	120	76.8	59163	PASS
175	174	5	9	7.1	4216	PASS
176	174	95	105	99.6	58912	PASS
177	176	5	10	6.0	3547	PASS

m/z	Abundance
35.90	146.0
36.50	130.0
37.20	131.0
39.90	1012.0
41.60	114.0
42.60	150.0
44.00	805.0
45.40	161.0
50.30	107.0
58.10	109.0
76.80	136.0
77.10	184.0
207.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
35.90	710.0
37.00	3146.0
38.00	2923.0
39.00	1315.0
39.90	1101.0
41.10	110.0
44.00	898.0
45.00	565.0
45.80	210.0
46.90	704.0
48.00	362.0
49.10	3327.0
50.10	12823.0
51.10	4675.0
52.00	228.0
53.00	133.0
53.90	127.0
55.00	229.0
56.00	1315.0
57.10	1951.0
59.10	120.0
60.10	769.0
61.10	3709.0
62.00	3507.0
63.10	3473.0
64.00	722.0
65.00	634.0
65.90	121.0
67.00	282.0
68.00	7425.0
69.00	7169.0
70.00	541.0
72.10	511.0
73.00	3795.0
74.10	12347.0
75.00	35944.0
76.10	3174.0
77.10	542.0
77.90	282.0
79.00	3440.0
80.00	1106.0
81.00	3699.0
82.00	735.0
83.00	142.0
87.00	3587.0
87.90	2951.0
90.80	375.0
92.00	2497.0
93.00	3447.0
94.00	9013.0
95.10	73008.0
96.10	4995.0
97.10	190.0
102.80	121.0
104.00	428.0
105.00	272.0
105.90	348.0
107.80	109.0
113.00	155.0
115.70	229.0
116.20	189.0
116.90	765.0
117.90	281.0
118.90	593.0
127.90	287.0
128.70	134.0
130.00	273.0
135.10	143.0
140.90	603.0
141.90	167.0
143.10	1285.0
143.90	114.0
144.90	766.0
145.90	222.0
148.00	171.0
149.00	106.0
154.80	138.0
161.10	120.0
171.10	401.0
172.00	797.0
173.10	949.0
174.00	56304.0
175.10	3997.0
176.00	54752.0
177.00	3560.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
35.90	823.0
37.00	3206.0
38.00	2858.0
39.00	1410.0
39.90	1102.0
41.10	137.0
44.00	937.0
45.00	621.0
45.90	197.0
46.90	787.0
48.00	430.0
49.10	3537.0
50.10	13794.0
51.10	4730.0
52.00	214.0
53.00	127.0
53.90	167.0
55.00	270.0
56.10	1345.0
57.10	1986.0
58.20	106.0
59.00	111.0
60.10	739.0
61.10	4021.0
62.10	3692.0
63.10	3581.0
64.10	947.0
65.10	879.0
66.90	322.0
68.00	7327.0
69.00	7544.0
69.90	581.0
72.00	352.0
73.00	3777.0
74.10	12829.0
75.00	38960.0
76.10	3227.0
76.90	627.0
77.90	316.0
78.90	3891.0
80.00	1216.0
81.00	3951.0
81.90	940.0
83.00	199.0
87.00	3673.0
87.90	3379.0
90.80	468.0
92.10	2663.0
93.10	3483.0
94.00	9186.0
95.10	79344.0
96.10	5192.0
97.10	221.0
102.80	136.0
104.00	461.0
105.00	275.0
105.90	449.0
111.40	105.0
113.00	144.0
114.90	130.0
115.70	211.0
116.20	164.0
116.90	788.0
118.00	294.0
118.90	629.0
127.90	336.0
128.90	146.0
130.00	339.0
135.10	142.0
136.90	100.0
139.70	106.0
140.90	690.0
142.00	157.0
143.10	1494.0
143.90	129.0
145.00	789.0
145.90	241.0
148.00	196.0
149.00	139.0
153.10	160.0
154.80	117.0
156.90	130.0
161.10	101.0
171.00	381.0
172.00	905.0
173.10	1168.0
174.00	61112.0
175.10	4295.0
176.00	61144.0
177.00	3620.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
35.90	764.0
37.00	3076.0
38.10	2660.0
39.00	1408.0
39.90	1059.0
41.10	136.0
44.00	1005.0
45.10	639.0
46.20	168.0
47.00	878.0
48.00	451.0
49.10	3252.0
50.10	13387.0
51.00	4152.0
51.90	184.0
52.30	135.0
53.00	127.0
53.90	208.0
55.00	261.0
56.10	1192.0
57.00	1893.0
58.20	115.0
60.10	654.0
61.10	3759.0
62.10	3523.0
63.00	3248.0
64.10	981.0
65.10	1019.0
67.00	262.0
68.00	6480.0
69.00	7170.0
70.00	565.0
71.80	348.0
73.00	3390.0
74.00	12543.0
75.00	37824.0
76.10	3114.0
76.90	661.0
77.80	307.0
78.90	4029.0
80.00	1192.0
81.00	4241.0
81.90	992.0
83.00	193.0
86.10	156.0
87.00	3180.0
87.90	3238.0
90.80	541.0
92.10	2476.0
93.10	3346.0
94.00	8487.0
95.10	78608.0
96.10	4721.0
97.00	150.0
102.80	111.0
104.00	402.0
105.00	175.0
105.90	429.0
108.20	130.0
111.40	106.0
113.00	109.0
114.90	173.0
115.80	280.0
116.90	705.0
118.00	327.0
119.00	592.0
127.90	362.0
129.00	154.0
130.00	337.0
135.10	192.0
136.90	128.0
139.70	139.0
140.90	749.0
141.90	176.0
143.00	1568.0
145.00	829.0
145.90	255.0
148.00	244.0
149.00	122.0
152.00	129.0
153.10	181.0
155.20	120.0
156.90	147.0
158.90	127.0
170.90	387.0
172.00	1074.0
173.10	1251.0
174.00	60072.0
175.10	4357.0
176.00	60840.0
177.10	3460.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205