

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007487.D
 Acq On : 12 Sep 2018 20:51
 Operator : SY/MD
 Sample : J4871-09
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KL9

Quant Time: Sep 13 06:54:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 02:33:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	125768	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	113208	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60158	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	36596	5.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.80%
7) Chloroethane-d5	1.58	69	27478	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.13	63	55824	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	3.96	46	70789	48.85	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.70%
24) Chloroform-d	4.41	84	66555	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.09	65	36180	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.20%
32) Benzene-d6	5.10	84	131303	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.13	67	39681	5.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.00%
41) Toluene-d8	7.36	98	133496	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
43) trans-1,3-Dichloropropene-	7.67	79	19475	5.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.20%
46) 2-Hexanone-d5	8.14	63	40837	45.12	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.24%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	27930	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	53201	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
34) Trichloroethene	5.97	95	1581	0.21 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007487.D
Acq On : 12 Sep 2018 20:51
Operator : SY/MD
Sample : J4871-09
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KL9

Quant Time: Sep 13 06:54:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 02:33:45 2018
Response via : Initial Calibration

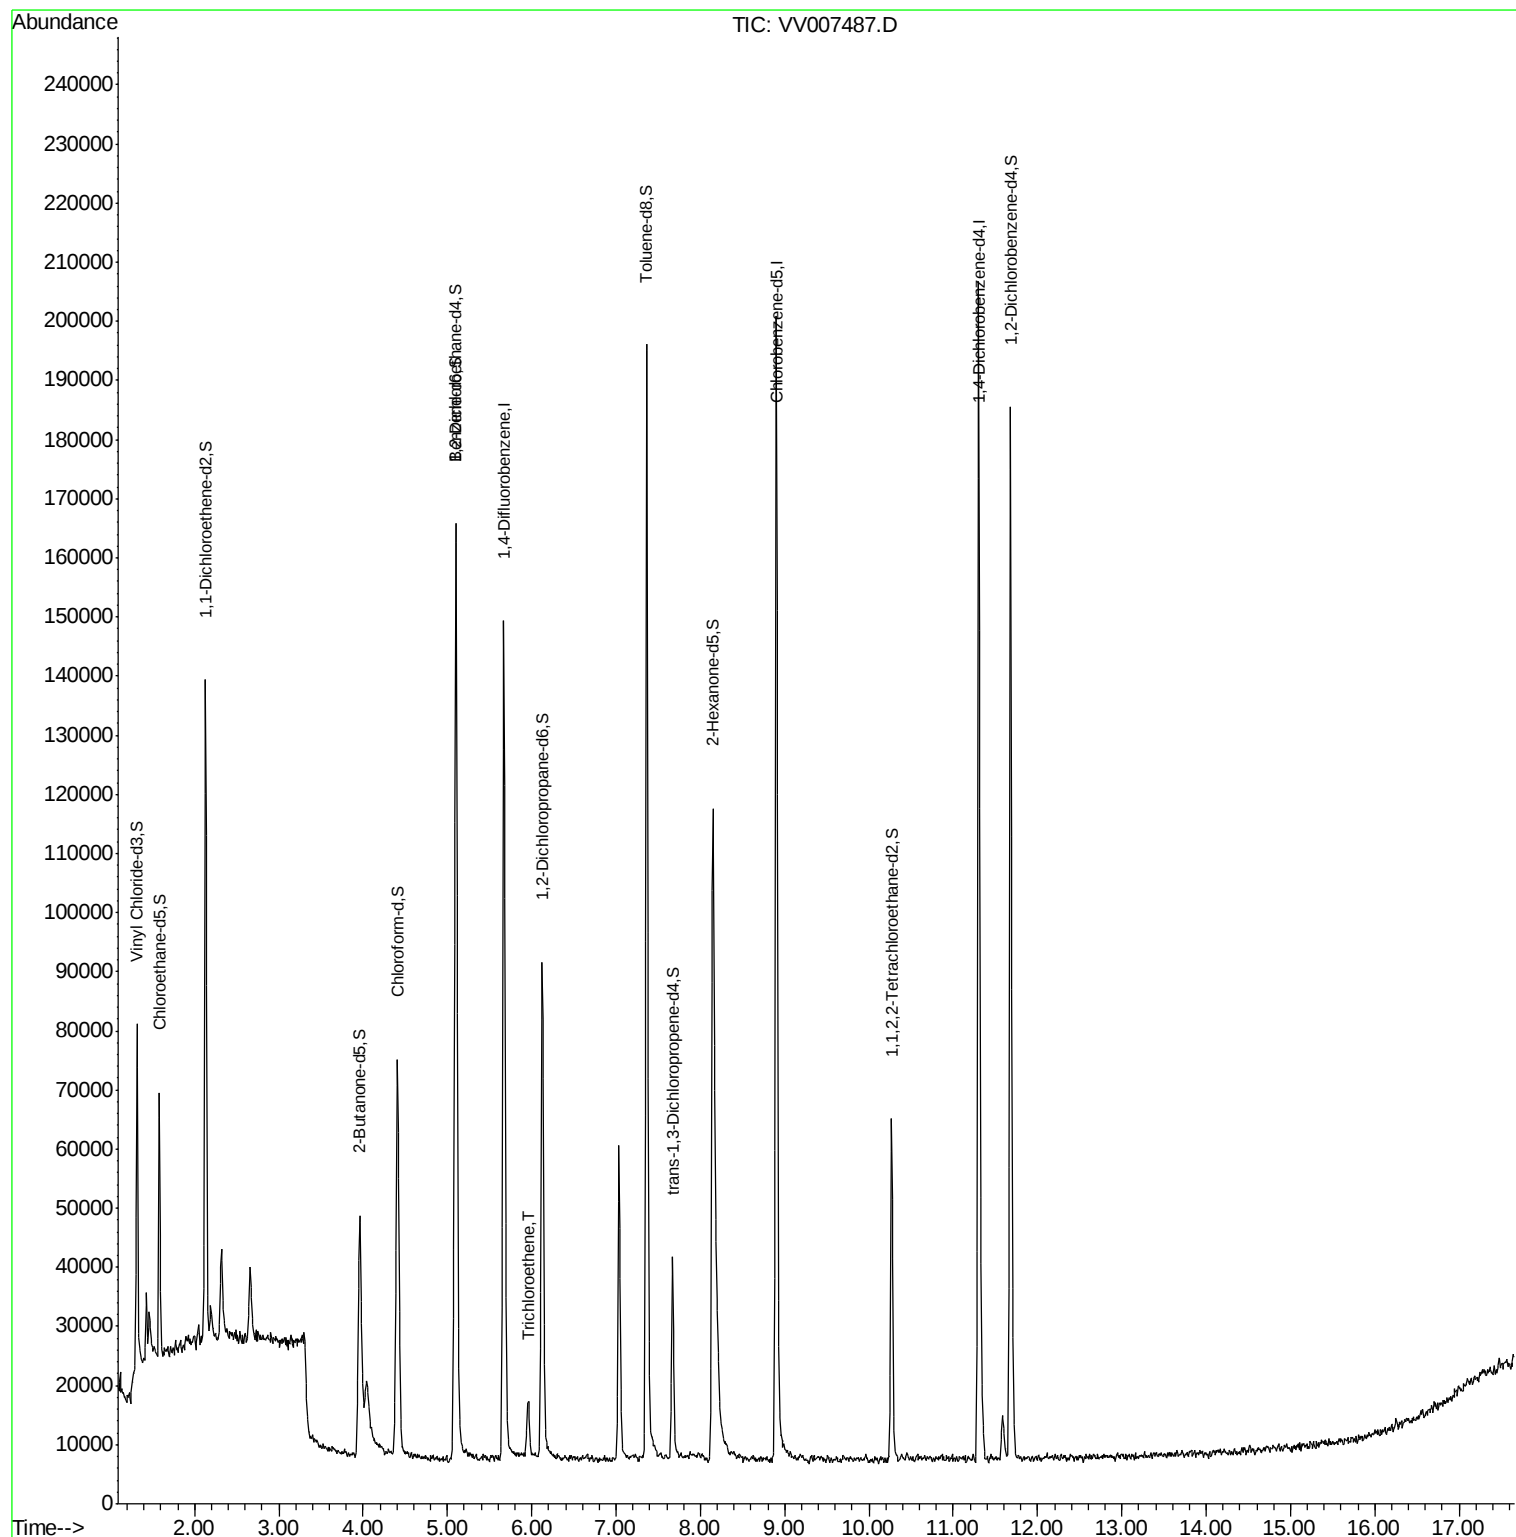

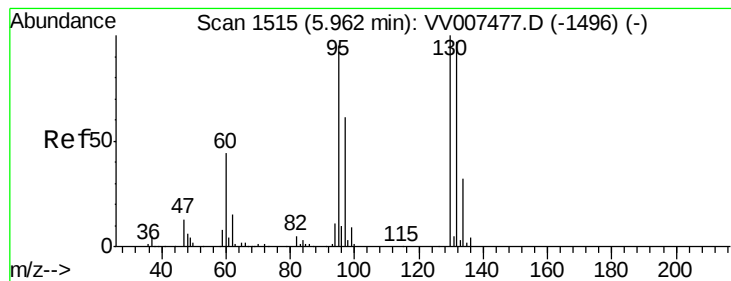

#34
 Trichloroethene
 Concen: 0.21 ug/L
 RT: 5.97 min Scan# 1517
 Delta R.T. 0.01 min
 Lab File: VV007487.D
 Acq: 12 Sep 2018 20:51

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KL9

Tot Ion:	95	Resp:	1581
Ion	Ratio	Lower	Upper
95	100		
97	74.8	42.8	79.4
132	93.8	67.6	125.6
130	79.6	69.6	129.2

