

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007488.D
 Acq On : 12 Sep 2018 21:18
 Operator : SY/MD
 Sample : J4871-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KM1

Quant Time: Sep 13 06:55:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 02:33:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	124667	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	112001	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58728	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35382	5.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.00%
7) Chloroethane-d5	1.58	69	26463	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.60%
11) 1,1-Dichloroethene-d2	2.13	63	54938	4.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.80%
20) 2-Butanone-d5	3.96	46	69210	48.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.36%
24) Chloroform-d	4.41	84	66097	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.09	65	34984	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.10	84	131233	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
36) 1,2-Dichloropropane-d6	6.13	67	38872	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	7.37	98	130892	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
43) trans-1,3-Dichloropropene-	7.67	79	18833	5.00	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.00%
46) 2-Hexanone-d5	8.15	63	37983	42.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.84%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	28947	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	52744	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	5478	0.74 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007488.D
Acq On : 12 Sep 2018 21:18
Operator : SY/MD
Sample : J4871-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KM1

Quant Time: Sep 13 06:55:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 02:33:45 2018
Response via : Initial Calibration

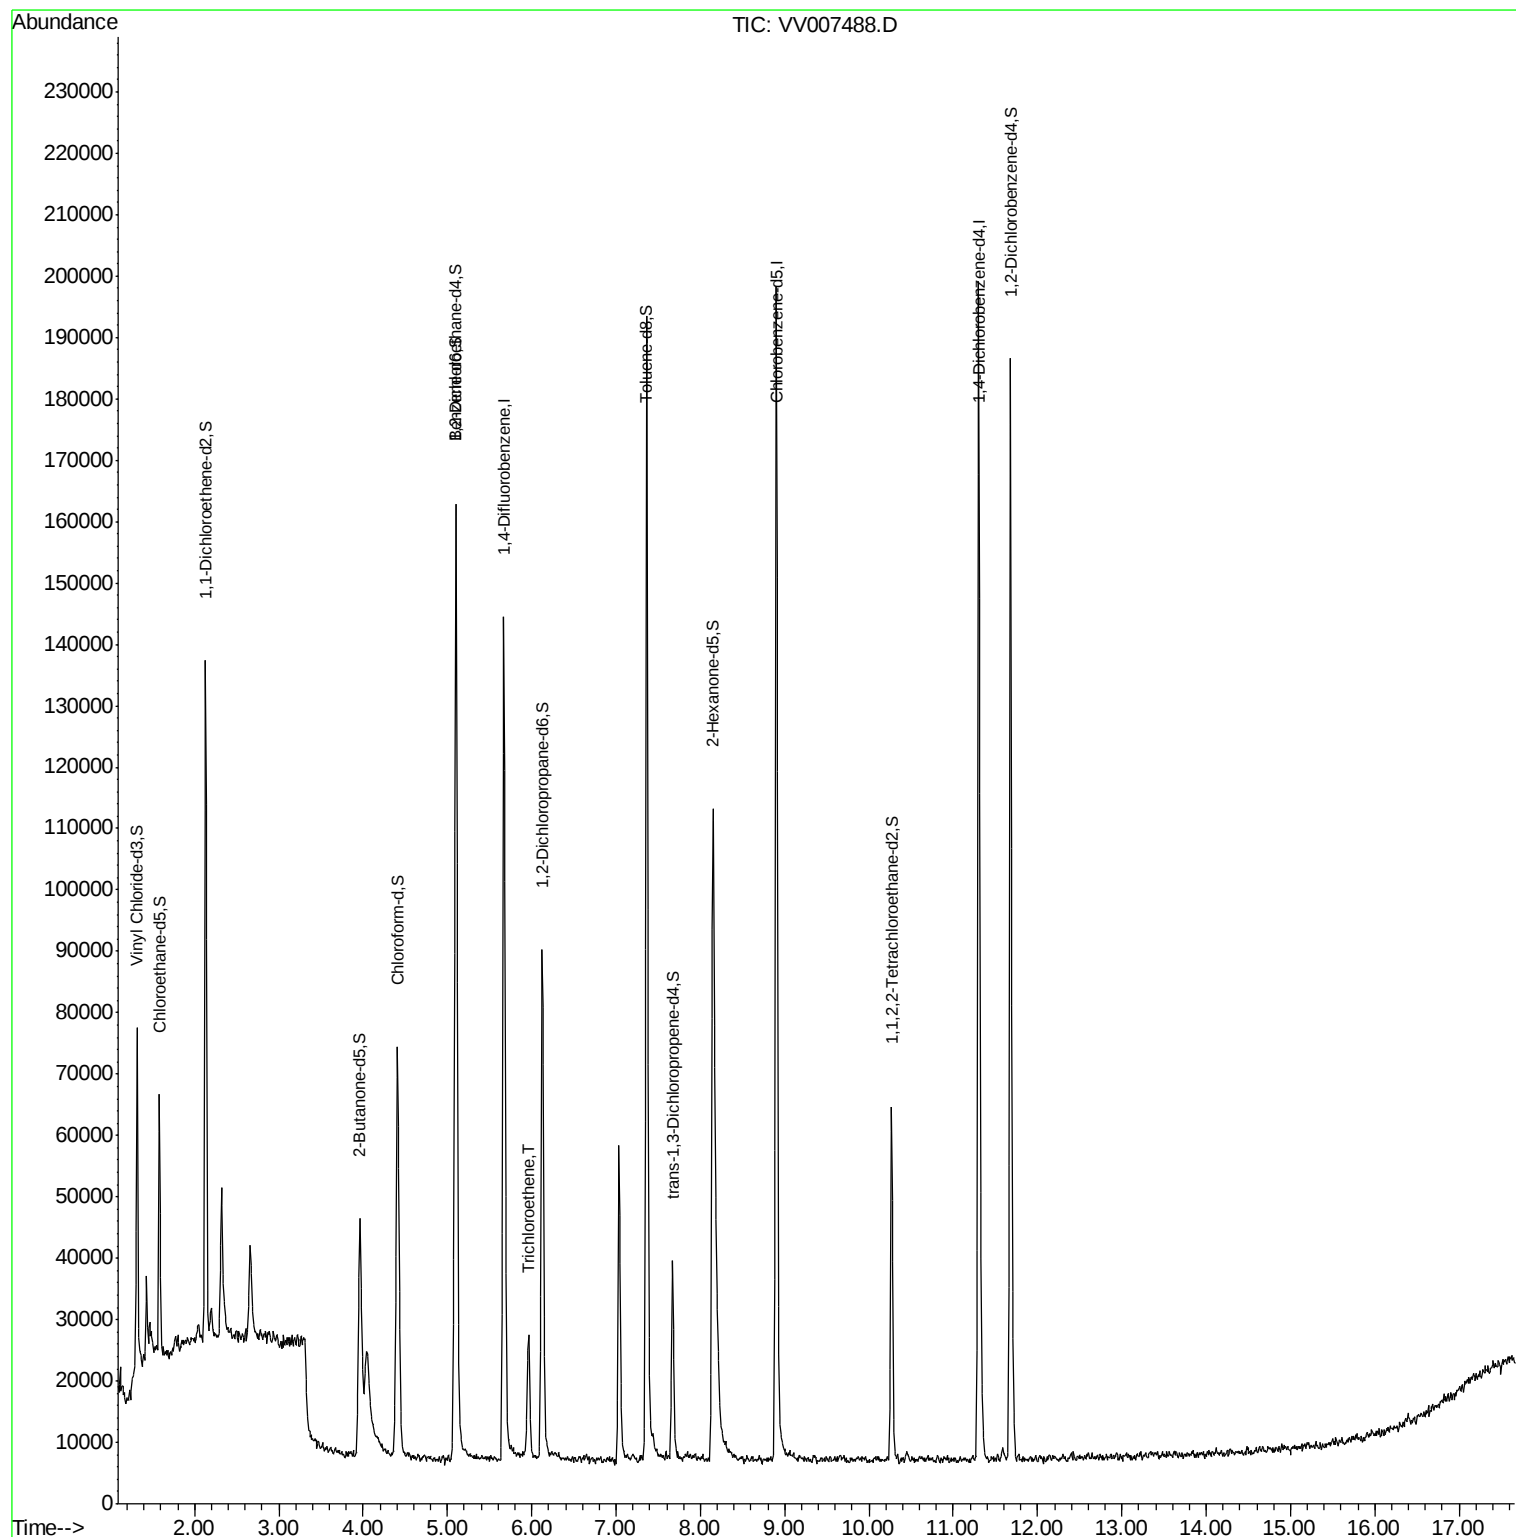

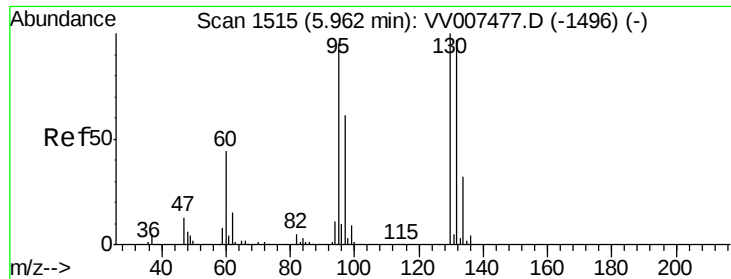

#34
 Trichloroethene
 Concen: 0.74 ug/L
 RT: 5.96 min Scan# 1516
 Delta R.T. 0.00 min
 Lab File: VV007488.D
 Acq: 12 Sep 2018 21:18

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KM1

Tot Ion:	95	Resp:	5478
Ion	Ratio	Lower	Upper
95	100		
97	61.8	42.8	79.4
132	90.4	67.6	125.6
130	101.7	69.6	129.2

