

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007490.D
 Acq On : 12 Sep 2018 22:13
 Operator : SY/MD
 Sample : J4871-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KM4

Quant Time: Sep 13 09:13:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 02:33:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	127707	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	115985	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60156	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35547	5.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.00%
7) Chloroethane-d5	1.58	69	26601	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.80%
11) 1,1-Dichloroethene-d2	2.13	63	54433	3.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.20%
20) 2-Butanone-d5	3.96	46	67031	45.55	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.10%
24) Chloroform-d	4.41	84	64194	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.09	65	34502	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
32) Benzene-d6	5.10	84	129945	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.13	67	37513	4.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.00%
41) Toluene-d8	7.36	98	130014	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloropropene-	7.67	79	17711	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.14	63	35280	38.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.10%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	26708	4.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	50878	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	28319	3.71 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007490.D
Acq On : 12 Sep 2018 22:13
Operator : SY/MD
Sample : J4871-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0KM4

Quant Time: Sep 13 09:13:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 02:33:45 2018
Response via : Initial Calibration

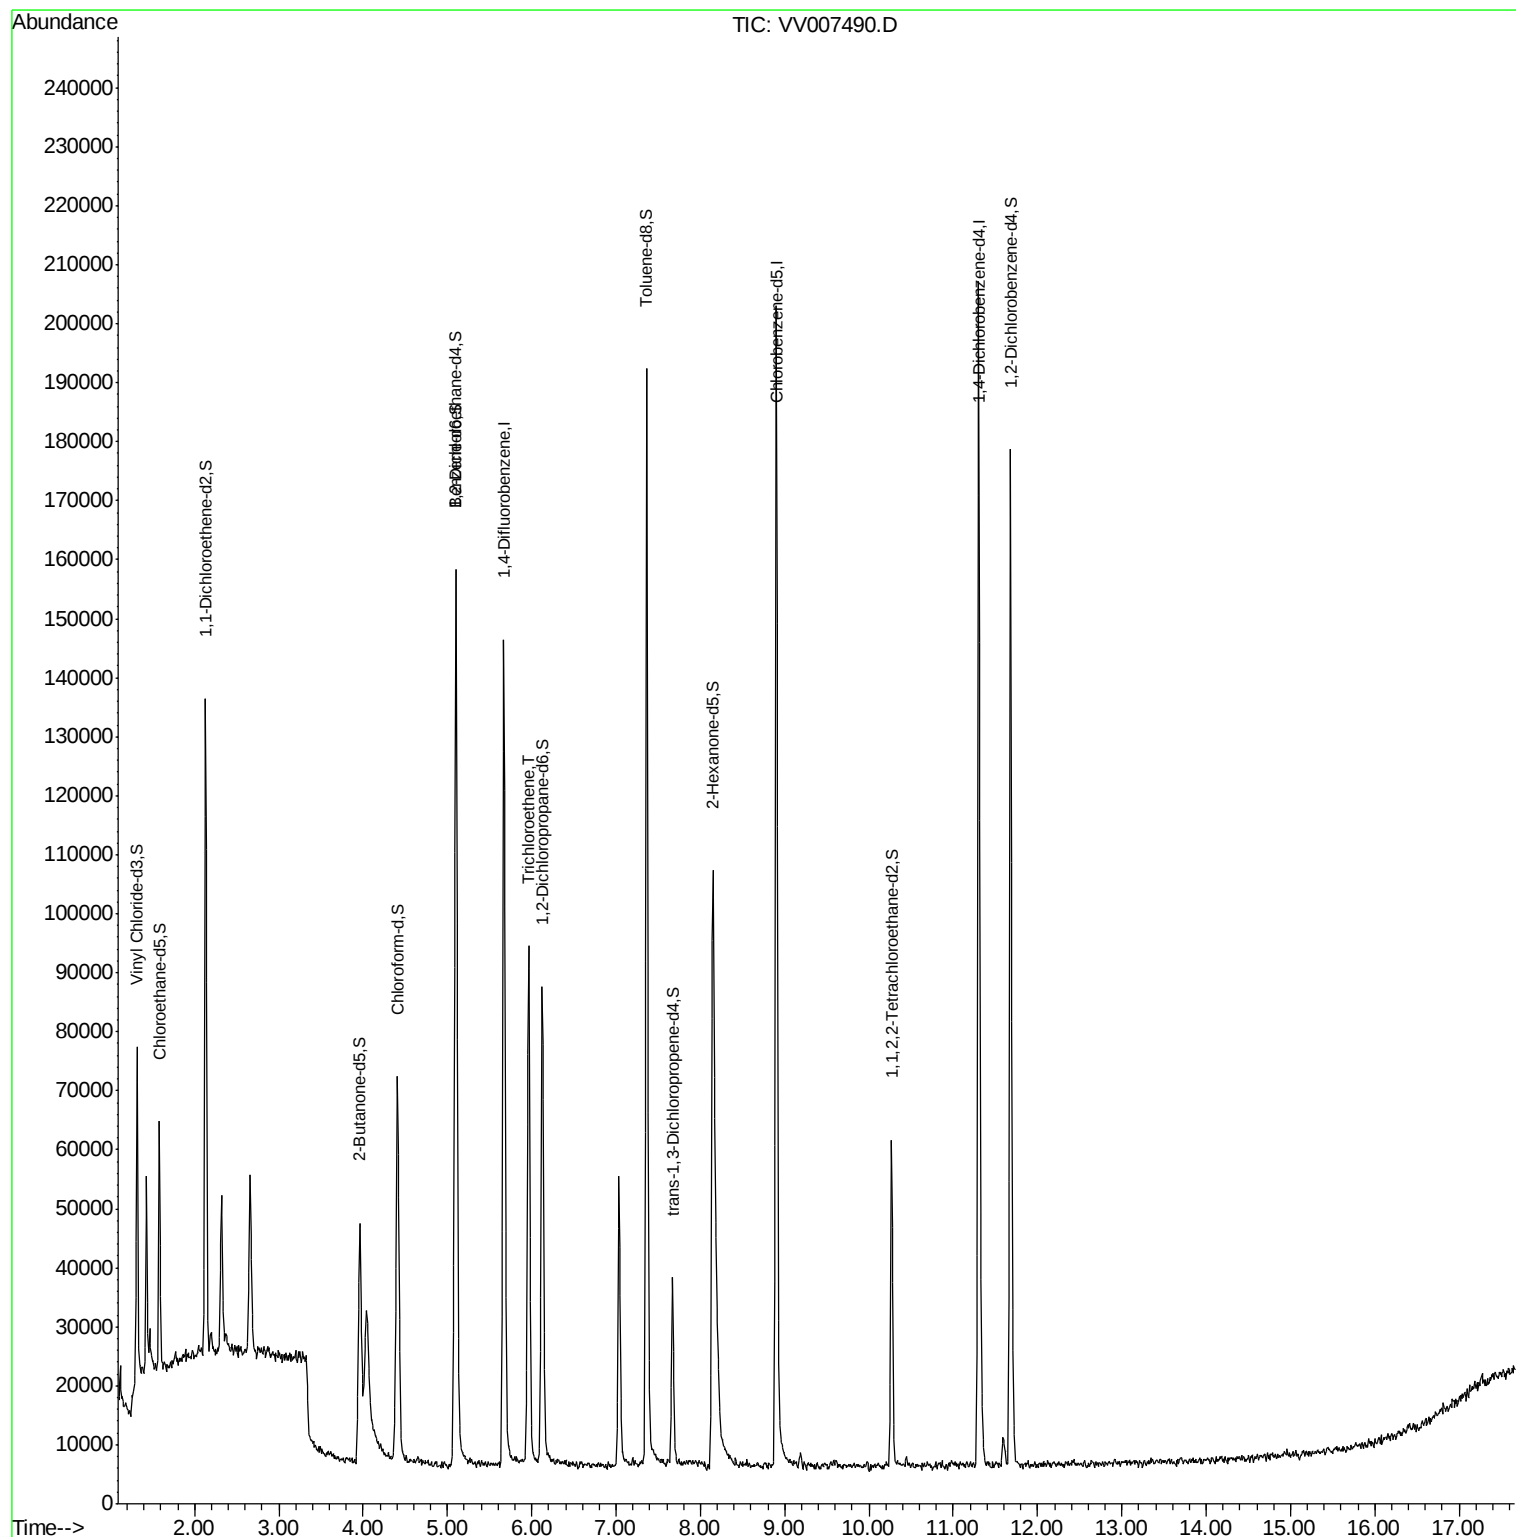

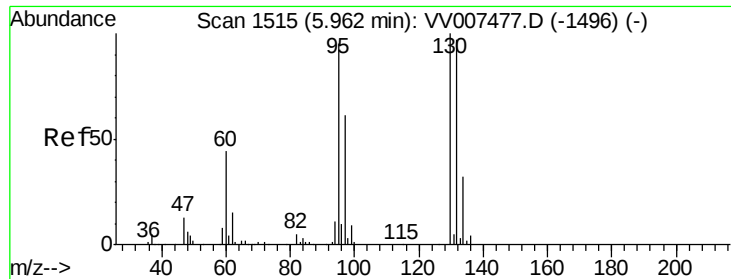

#34
 Trichloroethene
 Concen: 3.71 ug/L
 RT: 5.96 min Scan# 1516
 Delta R.T. 0.00 min
 Lab File: VV007490.D
 Acq: 12 Sep 2018 22:13

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KM4

Tot Ion:	95	Resp:	28319
Ion	Ratio	Lower	Upper
95	100		
97	64.9	42.8	79.4
132	105.4	67.6	125.6
130	105.8	69.6	129.2

