

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091218\
 Data File : VV007493.D
 Acq On : 12 Sep 2018 23:35
 Operator : SY/MD
 Sample : J4871-15
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KM9

Quant Time: Sep 18 02:42:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 02:33:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	122394	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	112837	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58482	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34414	5.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.20%
7) Chloroethane-d5	1.58	69	26125	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.20%
11) 1,1-Dichloroethene-d2	2.13	63	52520	3.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.60%
20) 2-Butanone-d5	3.96	46	66565	47.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.40%
24) Chloroform-d	4.41	84	62842	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.09	65	33971	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
32) Benzene-d6	5.10	84	124648	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	6.13	67	37628	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.36	98	126833	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
43) trans-1,3-Dichloropropene-	7.67	79	18116	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.14	63	37491	41.56	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.12%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	27254	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	49998	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Qvalue
34) Trichloroethene	5.96	95	7841	1.056 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV091218\
Data File : VV007493.D
Acq On : 12 Sep 2018 23:35
Operator : SY/MD
Sample : J4871-15
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KM9

Quant Time: Sep 18 02:42:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 02:33:45 2018
Response via : Initial Calibration

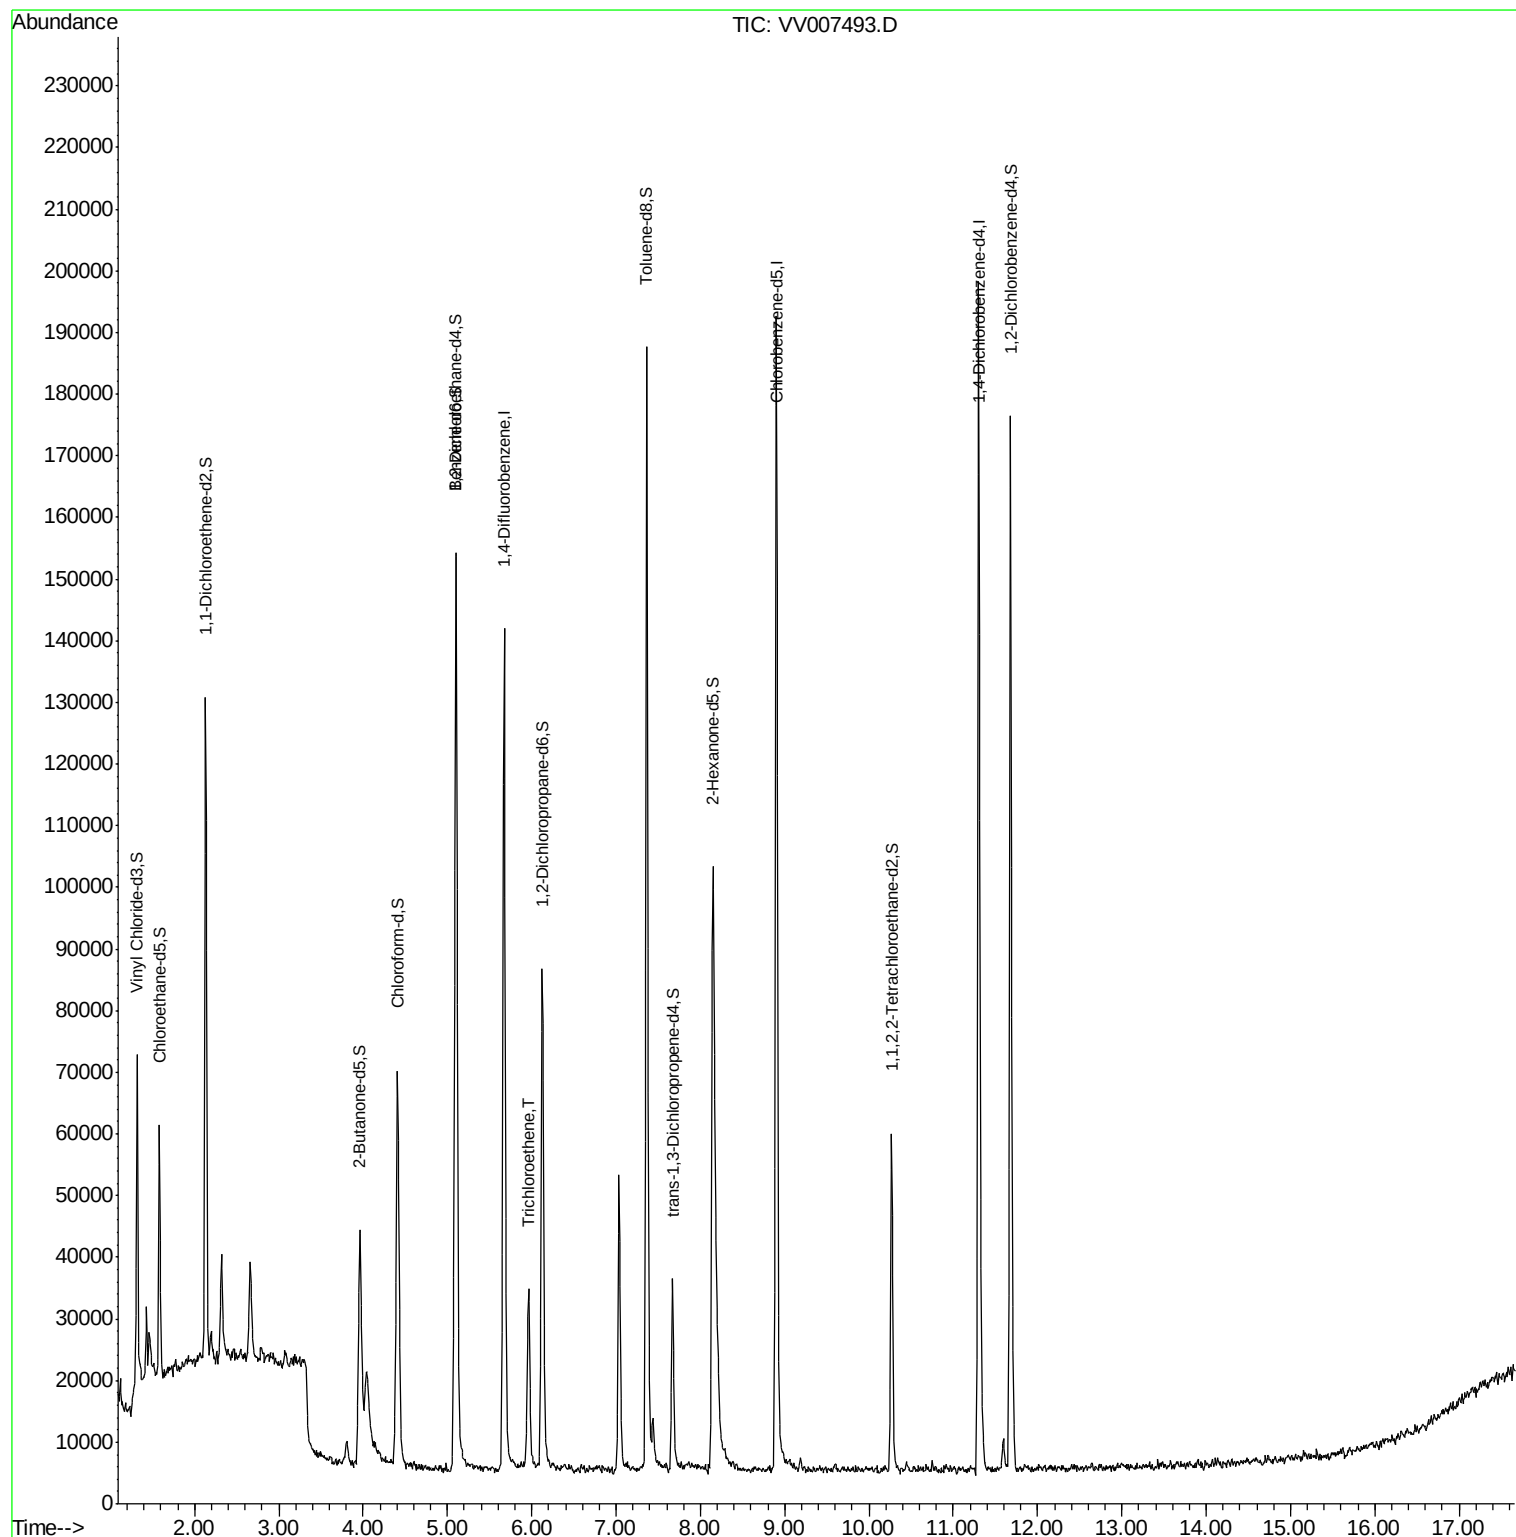

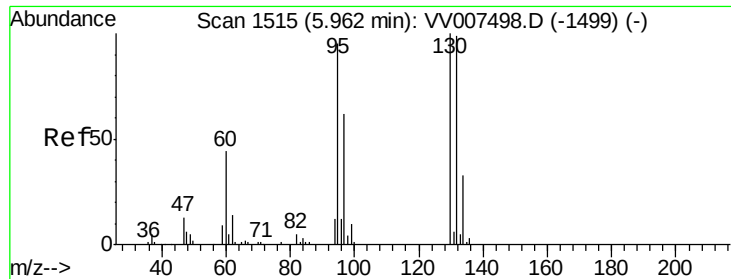

#34
 Trichloroethene
 Concen: 1.056 ug/L
 RT: 5.96 min Scan# 1516
 Delta R.T. 0.00 min
 Lab File: VV007493.D
 Acq: 12 Sep 2018 23:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KM9

Tgt Ion:	95	Resp:	7841
Ion	Ratio	Lower	Upper
95	100		
97	71.6	42.8	79.4
132	110.4	67.6	125.6
130	115.4	69.6	129.2

