

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007495.D
 Acq On : 13 Sep 2018 00:29
 Operator : SY/MD
 Sample : J4871-17
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KN2

Quant Time: Sep 13 07:10:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 02:33:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	124557	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	113698	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59180	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34750	5.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.20%
7) Chloroethane-d5	1.58	69	26252	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.00%
11) 1,1-Dichloroethene-d2	2.13	63	54294	4.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.80%
20) 2-Butanone-d5	3.96	46	64203	44.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.46%
24) Chloroform-d	4.41	84	63162	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
26) 1,2-Dichloroethane-d4	5.09	65	34275	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.10	84	127972	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.13	67	38587	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.36	98	128112	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
43) trans-1,3-Dichloropropene-	7.67	79	18274	4.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.60%
46) 2-Hexanone-d5	8.14	63	36135	39.75	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.50%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	26473	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	52273	5.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.00%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	40905	5.47 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007495.D
Acq On : 13 Sep 2018 00:29
Operator : SY/MD
Sample : J4871-17
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KN2

Quant Time: Sep 13 07:10:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 02:33:45 2018
Response via : Initial Calibration

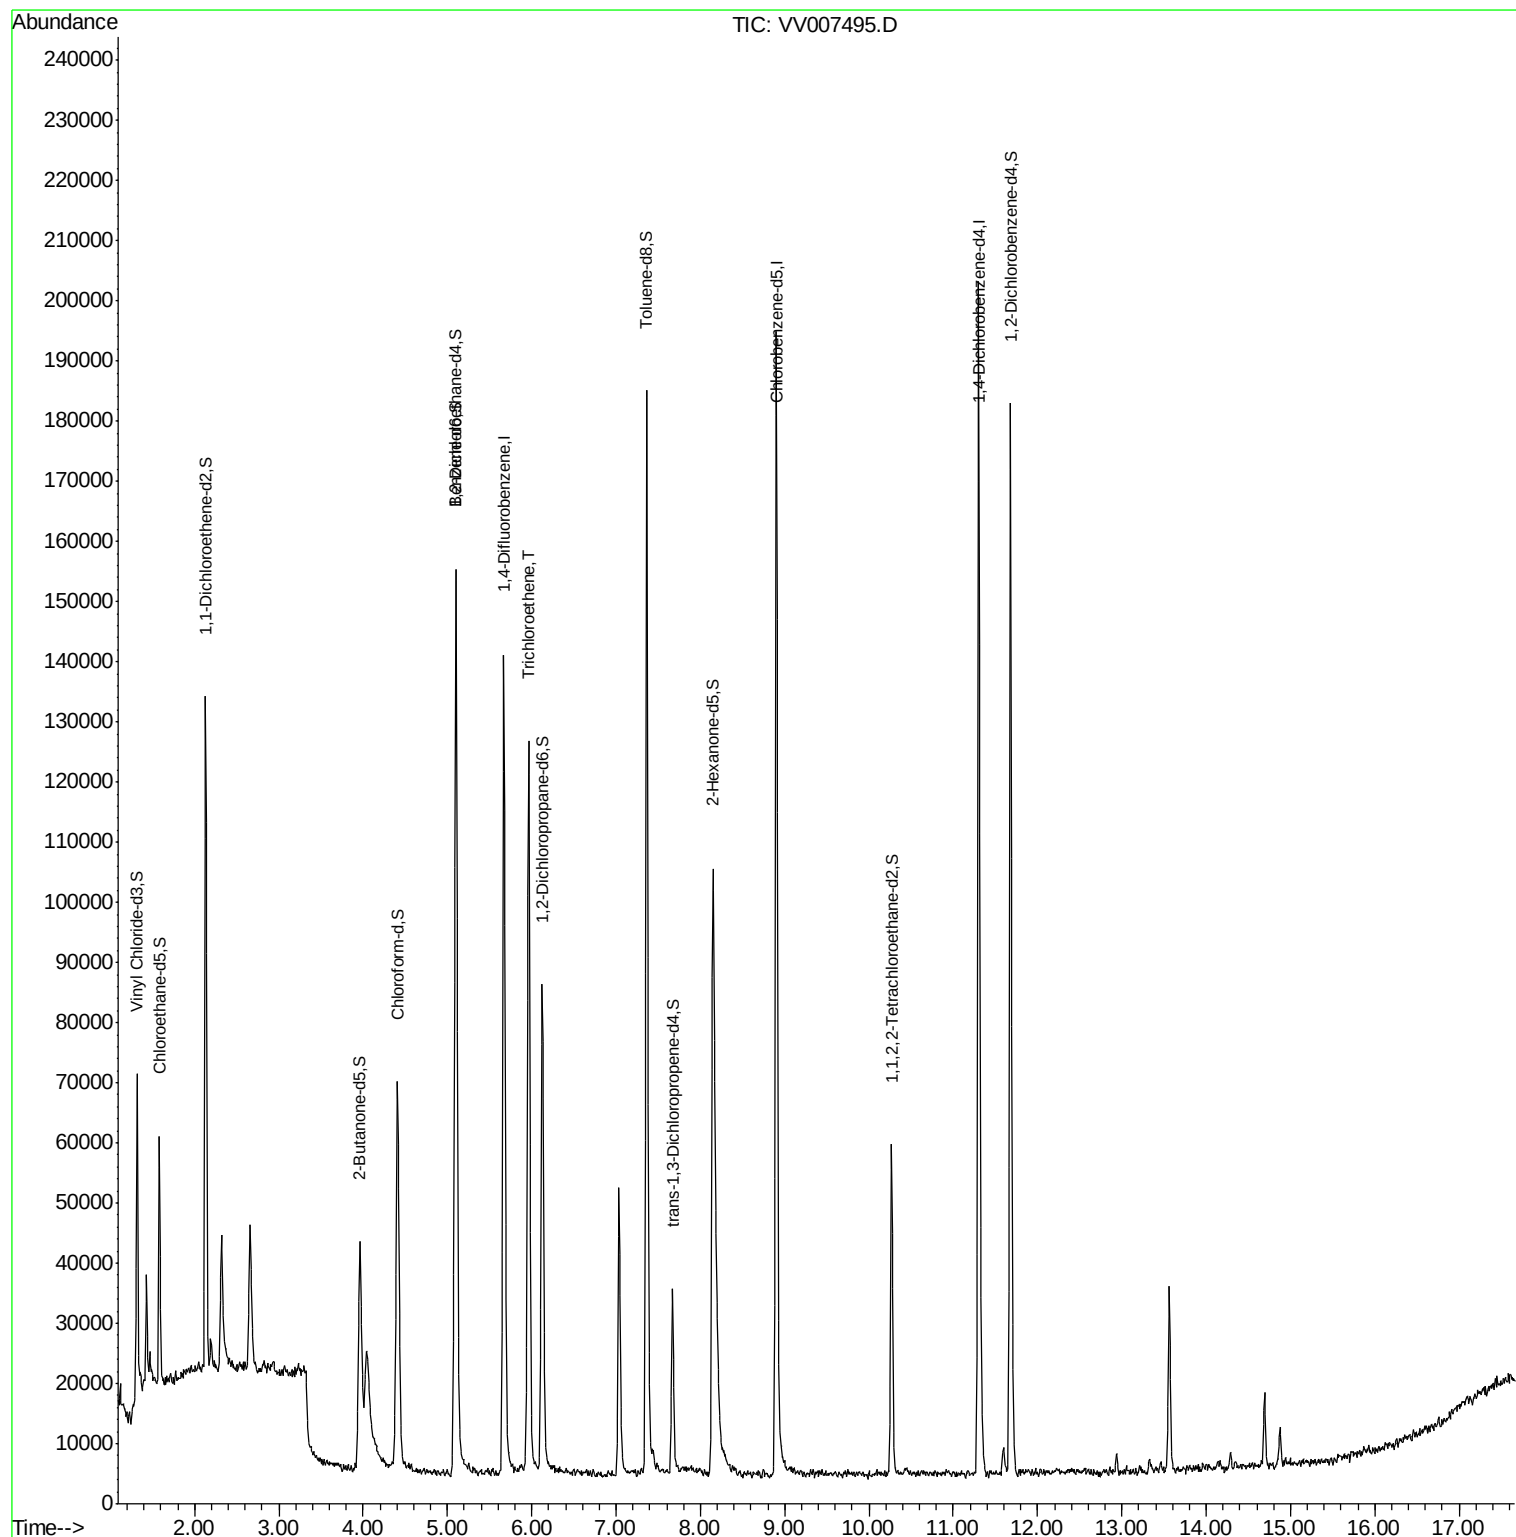

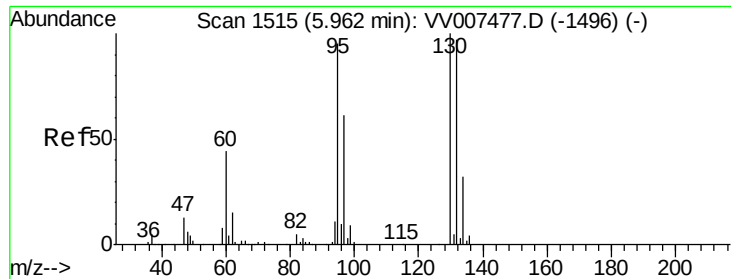

#34
 Trichloroethene
 Concen: 5.47 ug/L
 RT: 5.96 min Scan# 1516
 Delta R.T. 0.00 min
 Lab File: VV007495.D
 Acq: 13 Sep 2018 00:29

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KN2

Tot Ion:	95	Resp:	40905
Ion	Ratio	Lower	Upper
95	100		
97	64.4	42.8	79.4
132	101.8	67.6	125.6
130	106.6	69.6	129.2

