

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007497.D
 Acq On : 13 Sep 2018 01:24
 Operator : SY/MD
 Sample : J4871-19
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KN5

Quant Time: Sep 13 07:14:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 02:33:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	125160	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	112948	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60231	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	33510	5.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.00%
7) Chloroethane-d5	1.58	69	25927	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.13	63	50439	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.96	46	65141	45.17	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.34%
24) Chloroform-d	4.41	84	61583	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	5.09	65	33264	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.10	84	126121	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.13	67	37947	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.36	98	123864	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
43) trans-1,3-Dichloropropene-	7.67	79	16704	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.14	63	35238	39.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.04%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	25271	4.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	50530	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	10588	1.43 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007497.D
Acq On : 13 Sep 2018 01:24
Operator : SY/MD
Sample : J4871-19
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KN5

Quant Time: Sep 13 07:14:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 02:33:45 2018
Response via : Initial Calibration

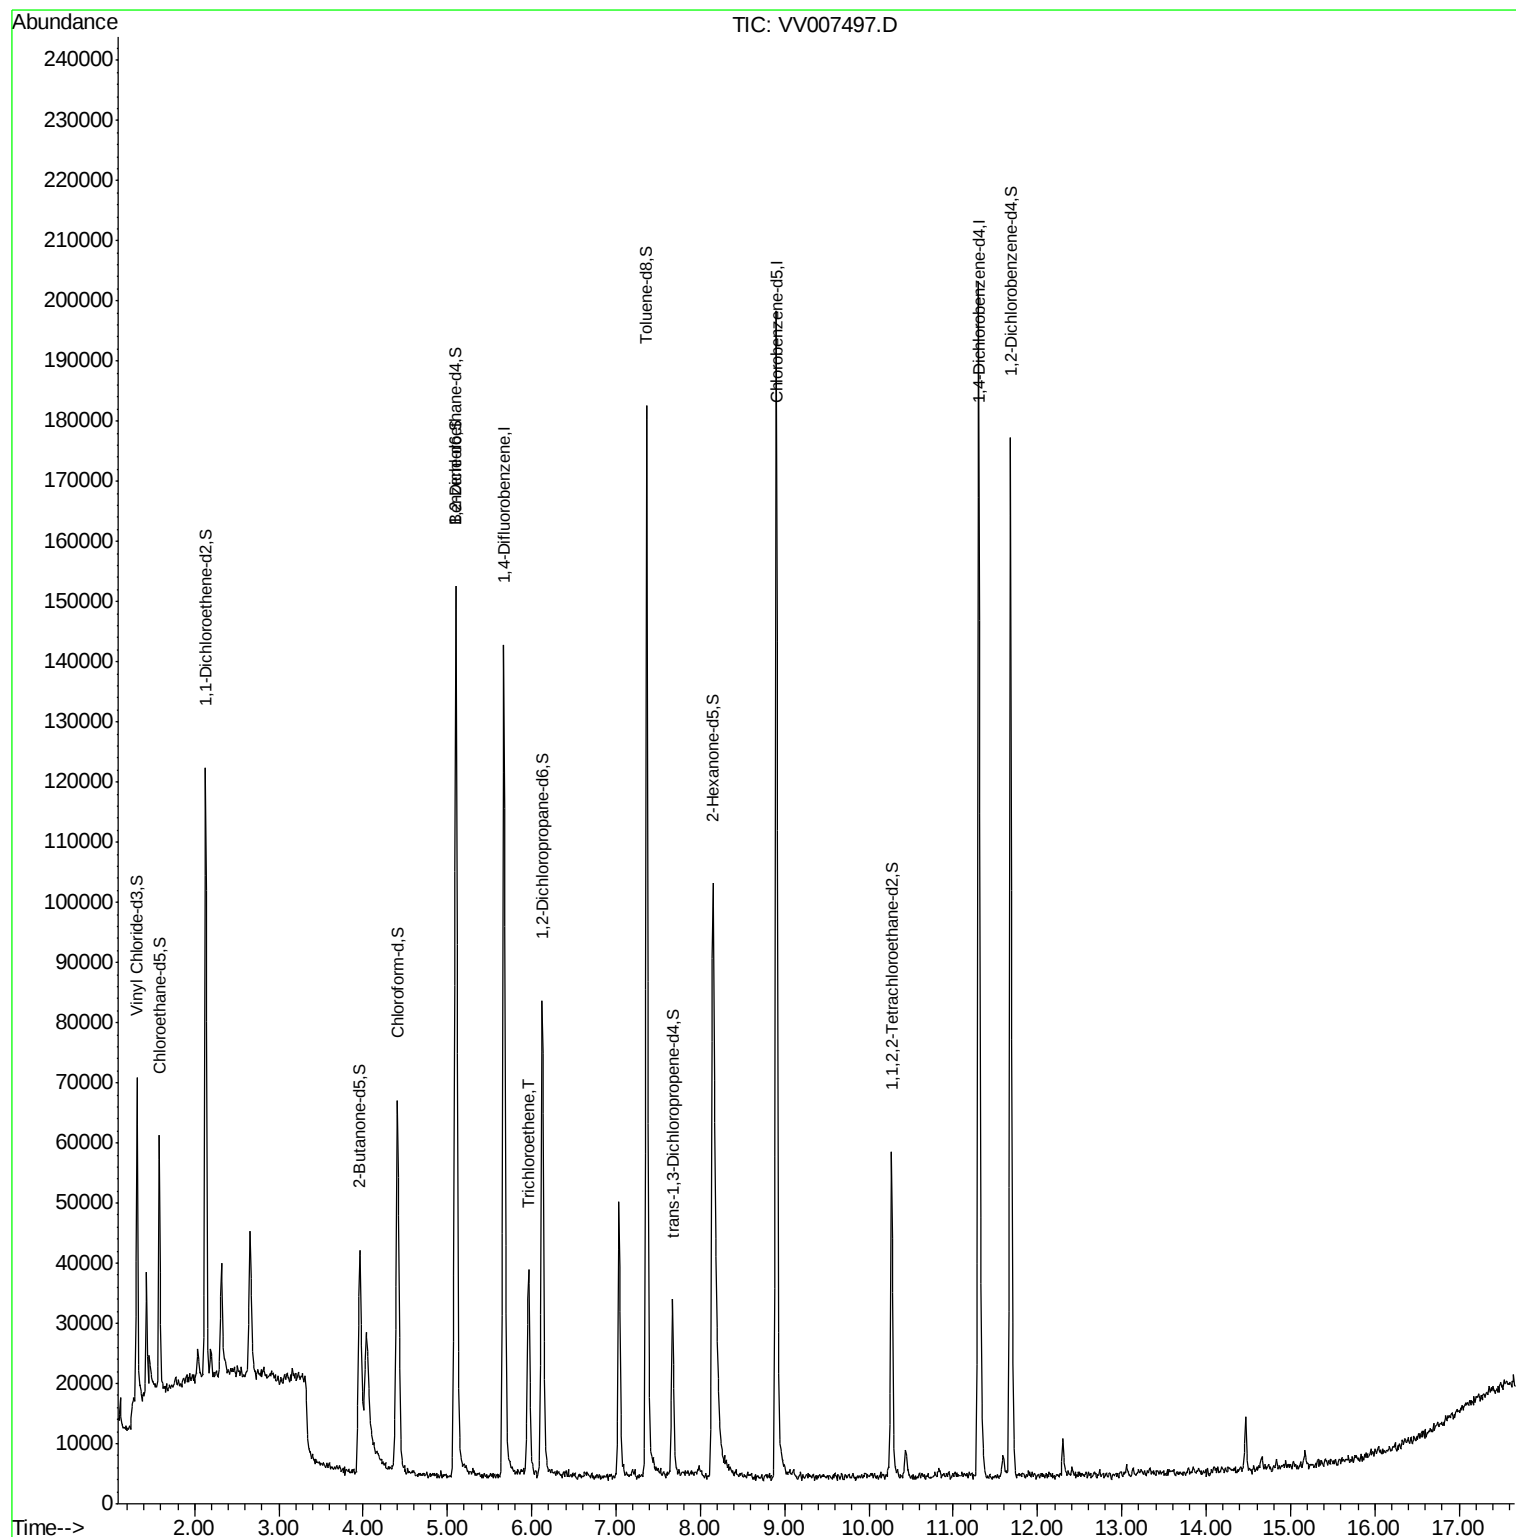

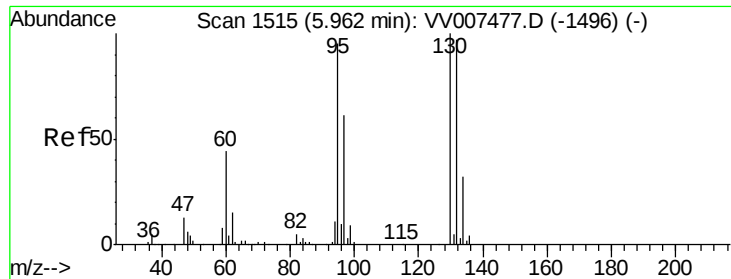

#34
 Trichloroethene
 Concen: 1.43 ug/L
 RT: 5.96 min Scan# 1515
 Delta R.T. 0.00 min
 Lab File: VV007497.D
 Acq: 13 Sep 2018 01:24

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KN5

Tot Ion:	95	Resp:	10588
Ion	Ratio	Lower	Upper
95	100		
97	60.1	42.8	79.4
132	101.5	67.6	125.6
130	98.6	69.6	129.2

