

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091218\
 Data File : VV007502.D
 Acq On : 13 Sep 2018 03:41
 Operator : SY/MD
 Sample : J4872-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KN8

Quant Time: Sep 13 07:33:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 13 07:19:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	121970	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	113266	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59144	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34046	5.22	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.40%
7) Chloroethane-d5	1.58	69	26339	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.20%
11) 1,1-Dichloroethene-d2	2.13	63	53123	4.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.80%
20) 2-Butanone-d5	3.96	46	67157	47.78	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.56%
24) Chloroform-d	4.41	84	63537	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.09	65	34383	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.00%
32) Benzene-d6	5.10	84	127955	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.40%
36) 1,2-Dichloropropane-d6	6.13	67	38061	4.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.80%
41) Toluene-d8	7.36	98	127919	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
43) trans-1,3-Dichloropropene-	7.67	79	17211	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.14	63	37025	40.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.78%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	26790	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	52506	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	10482	1.41 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091218\
Data File : VV007502.D
Acq On : 13 Sep 2018 03:41
Operator : SY/MD
Sample : J4872-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0KN8

Quant Time: Sep 13 07:33:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091218WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 13 07:19:10 2018
Response via : Initial Calibration

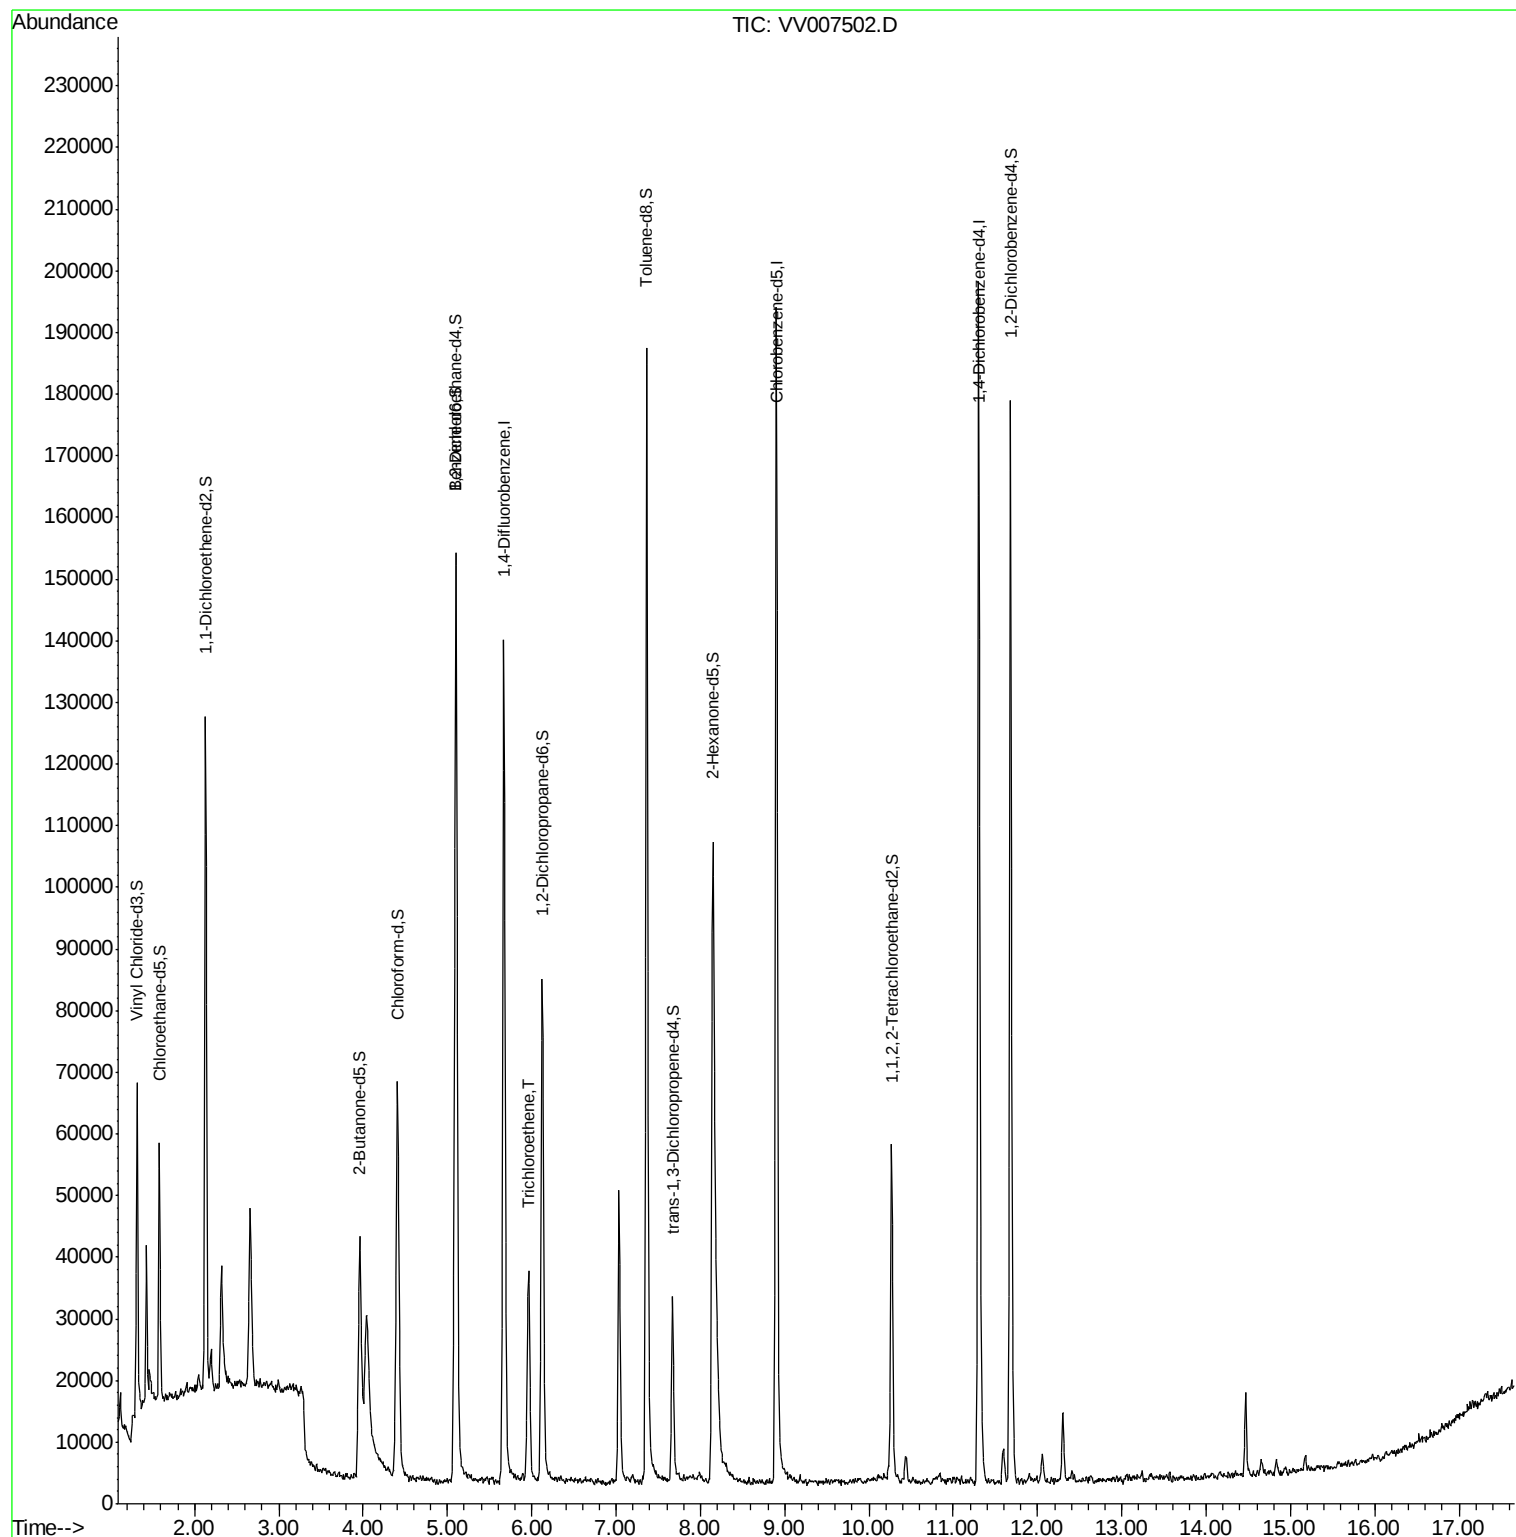

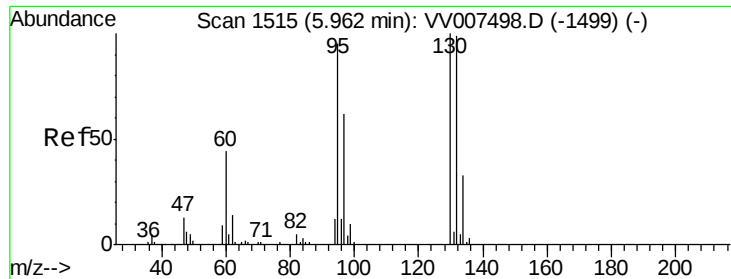

#34
 Trichloroethene
 Concen: 1.41 ug/L
 RT: 5.96 min Scan# 1516
 Delta R.T. 0.00 min
 Lab File: VV007502.D
 Acq: 13 Sep 2018 03:41

Instrument :
 MSVOA_V
 ClientSampleId :
 C0KN8

Tot Ion:	95	Resp:	10482
Ion	Ratio	Lower	Upper
95	100		
97	67.3	42.8	79.4
132	105.7	67.6	125.6
130	106.7	69.6	129.2

